

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
 Data File : VU054906.D
 Acq On : 28 Jul 2023 11:17
 Operator : MD/SY
 Sample : VU0728WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0728WBL01

Quant Time: Jul 28 23:11:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Jul 26 09:45:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	26054	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	7524	0.953	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	8762	0.982	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
Data File : VU054906.D
Acq On : 28 Jul 2023 11:17
Operator : MD/SY
Sample : VU0728WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0728WBL01


Quant Time: Jul 28 23:11:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Jul 26 09:45:35 2023
Response via : Initial Calibration

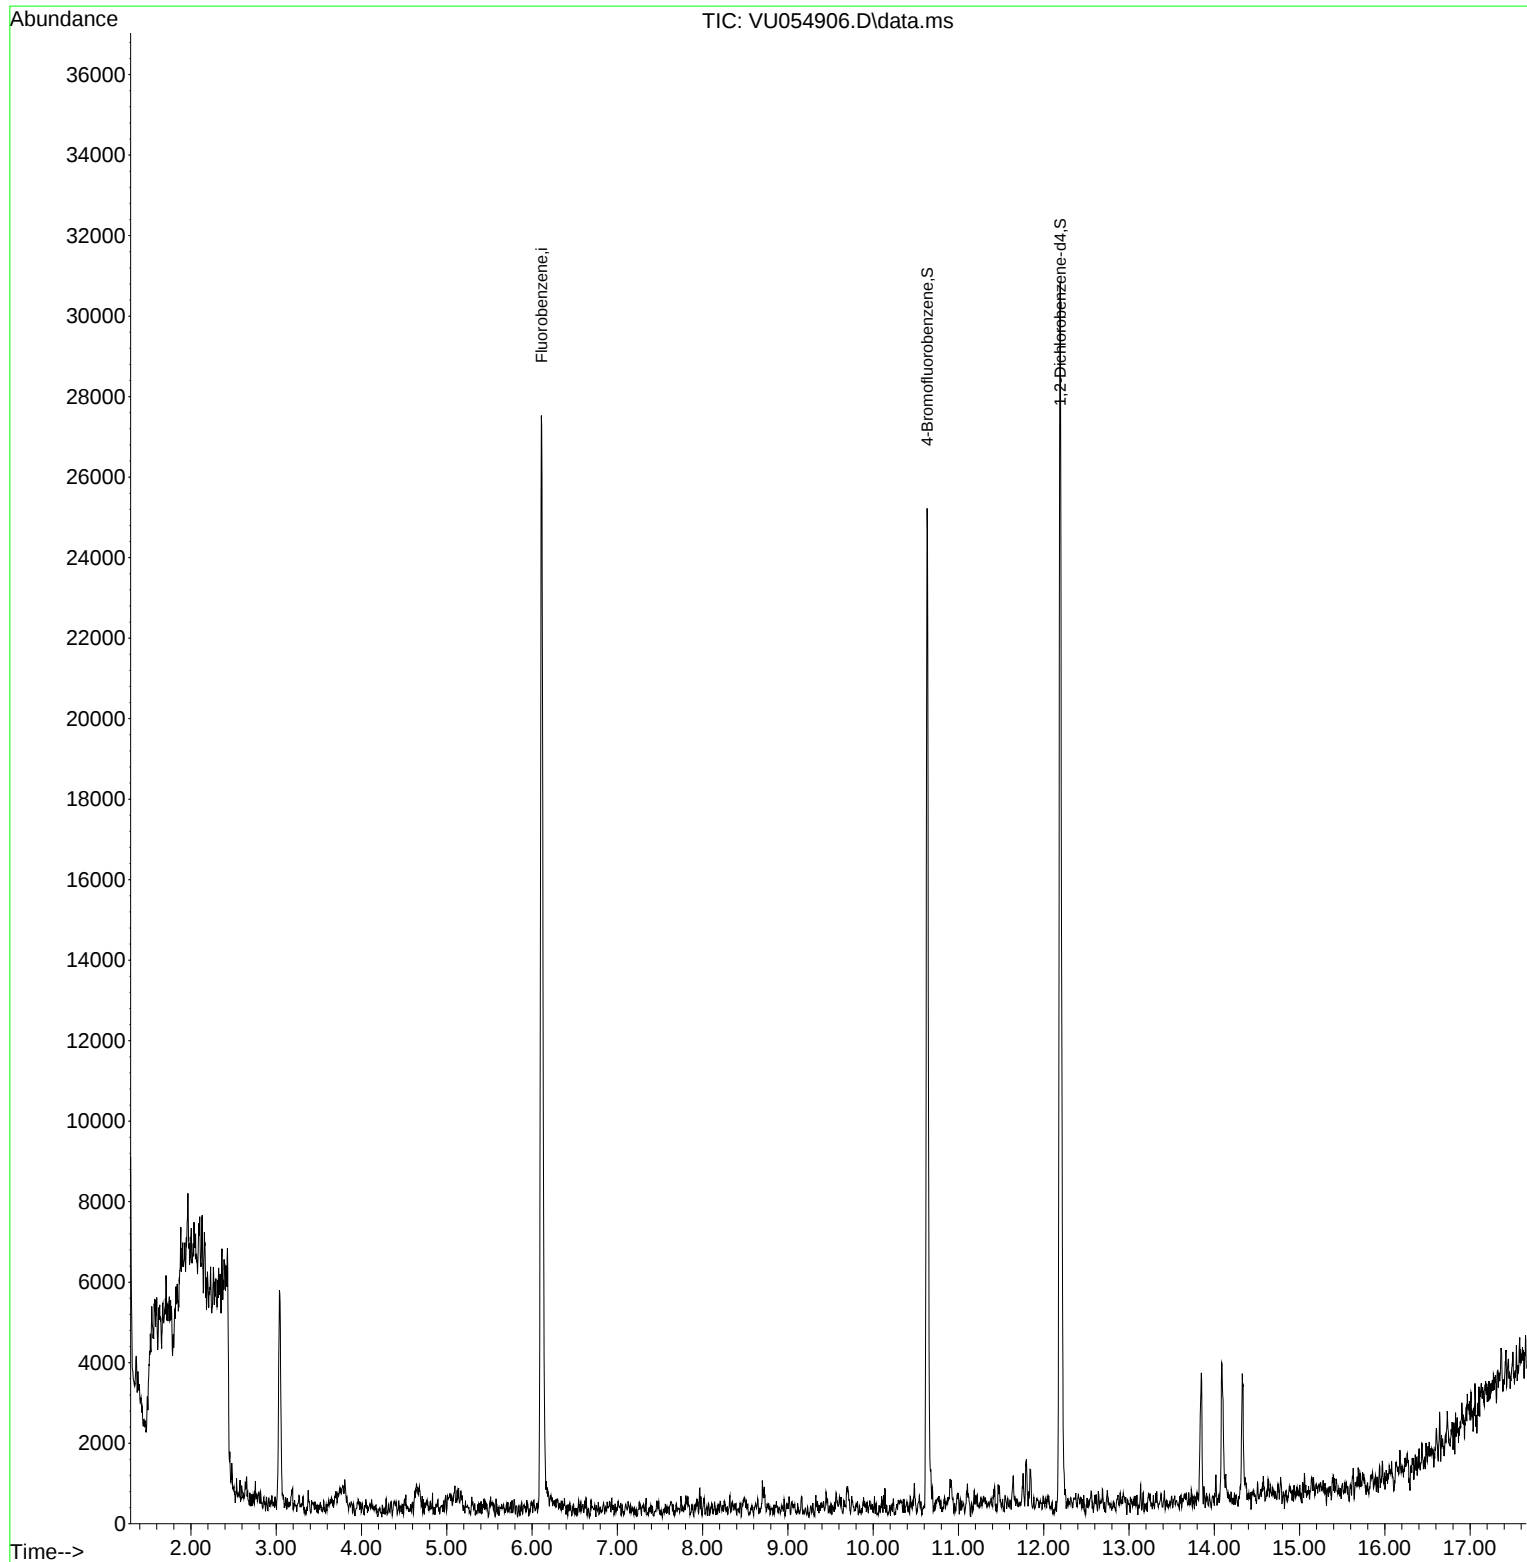



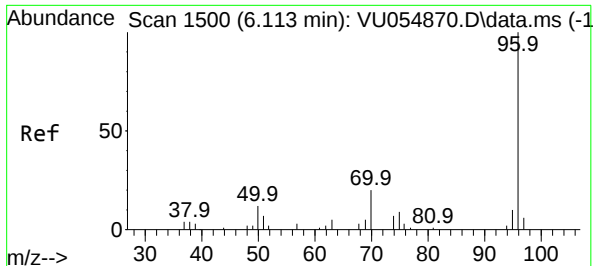


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU054906.D
Acq: 28 Jul 2023 11:17

Instrument :
MSVOA_U
ClientSampleId :
VU0728WBL01



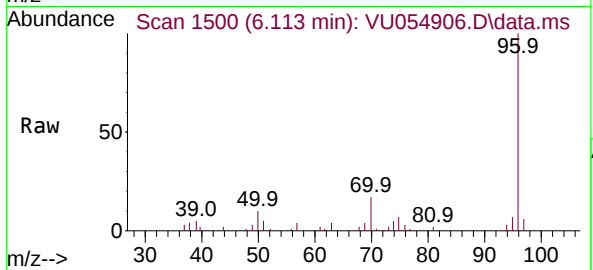



Tgt Ion:	96	Resp:	26054
Ion Ratio	Lower	Upper	
96	100		
70	18.1	14.0	21.0
95	8.6	8.7	13.1#
97	6.4	0.0	0.0#

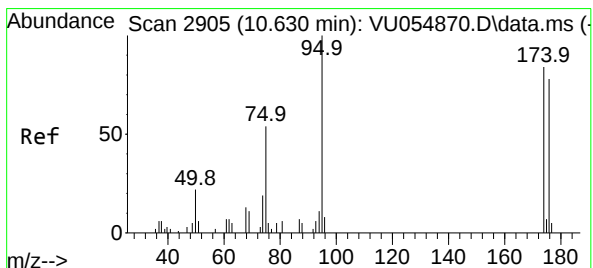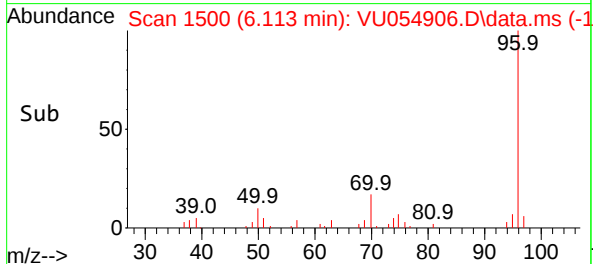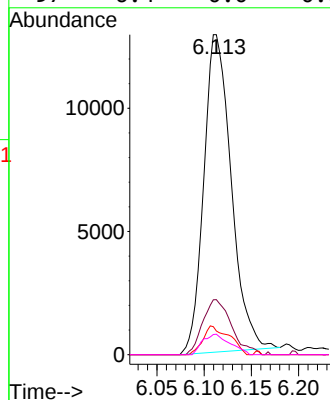

#57
4-Bromofluorobenzene
Concen: 0.953 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.003 min
Lab File: VU054906.D
Acq: 28 Jul 2023 11:17

Tgt Ion:	95	Resp:	7524
Ion Ratio	Lower	Upper	
95	100		
174	102.6	79.3	118.9
176	95.7	71.5	107.3

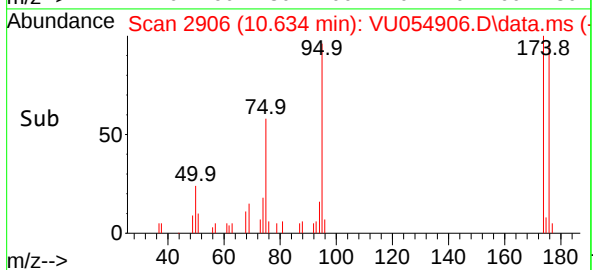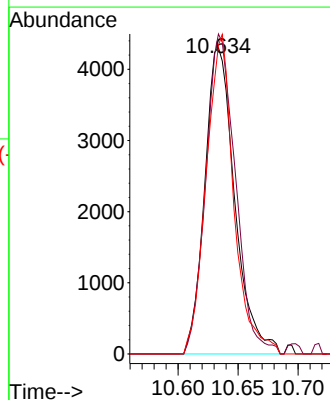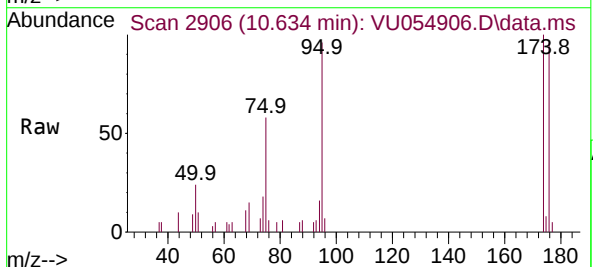

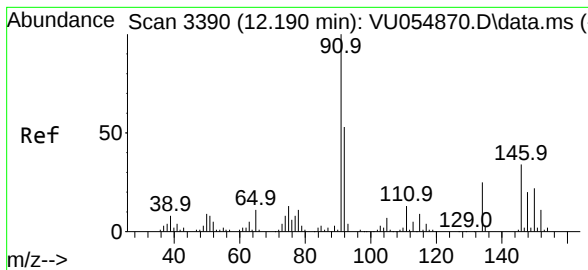

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.982 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU054906.D
 Acq: 28 Jul 2023 11:17

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0728WBL01

Tgt Ion:	152	Resp:	8762
Ion Ratio	Lower	Upper	
152	100		
115	55.1	0.0	234.8
150	148.1	0.0	598.2

