

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
 Data File : VU054906.D
 Acq On : 28 Jul 2023 11:17
 Operator : MD/SY
 Sample : VU0728WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0728WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	331	334	337	rBV5	1607	1187	2.06%	0.615%
2	3.039	533	544	554	rBV4	5447	9917	17.23%	5.137%
3	3.193	584	592	594	rVB4	545	668	1.16%	0.346%
4	5.097	1174	1184	1187	rBV4	487	576	1.00%	0.298%
5	6.110	1485	1499	1515	rBV	27272	54677	95.02%	28.323%
6	10.634	2897	2906	2918	rBV2	24822	40856	71.00%	21.164%
7	11.643	3212	3220	3224	rBV3	833	1051	1.83%	0.544%
8	11.759	3247	3256	3262	rVB3	815	884	1.54%	0.458%
9	11.791	3262	3266	3267	rBV2	1046	697	1.21%	0.361%
10	11.839	3277	3281	3291	rVB4	965	1192	2.07%	0.617%
11	12.193	3378	3391	3408	rBV2	30560	57540	100.00%	29.807%
12	12.746	3557	3563	3566	rBV	550	627	1.09%	0.325%
13	13.232	3709	3714	3717	rBV2	462	580	1.01%	0.300%
14	13.849	3896	3906	3913	rVV7	3280	5073	8.82%	2.628%
15	14.087	3972	3980	3993	rBV5	3478	6361	11.05%	3.295%
16	14.328	4049	4055	4057	rBV3	2891	2740	4.76%	1.419%
17	14.778	4190	4195	4200	rVV3	693	806	1.40%	0.418%
18	15.939	4551	4556	4558	rBV2	670	580	1.01%	0.300%
19	16.132	4609	4616	4621	rBV5	702	1113	1.93%	0.577%
20	16.357	4681	4686	4689	rBV3	623	583	1.01%	0.302%
21	16.604	4760	4763	4770	rVB5	821	836	1.45%	0.433%
22	16.643	4770	4775	4779	rVB4	1235	1029	1.79%	0.533%
23	16.733	4801	4803	4813	rVB6	919	861	1.50%	0.446%
24	16.830	4830	4833	4835	rBV3	1037	597	1.04%	0.309%
25	16.955	4866	4872	4874	rBV6	782	816	1.42%	0.423%
26	17.058	4902	4904	4907	rVB4	1077	605	1.05%	0.313%
27	17.325	4983	4987	4989	rBV3	683	593	1.03%	0.307%




Sum of corrected areas: 193045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
Data File : VU054906.D
Acq On : 28 Jul 2023 11:17
Operator : MD/SY
Sample : VU0728WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0728WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

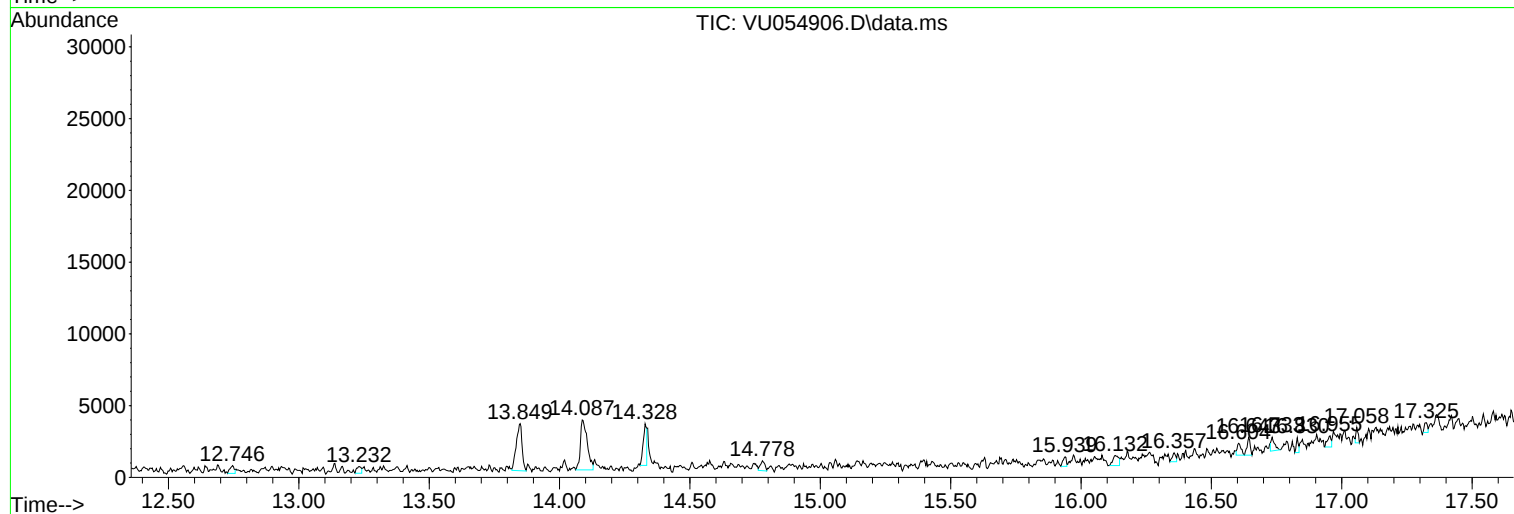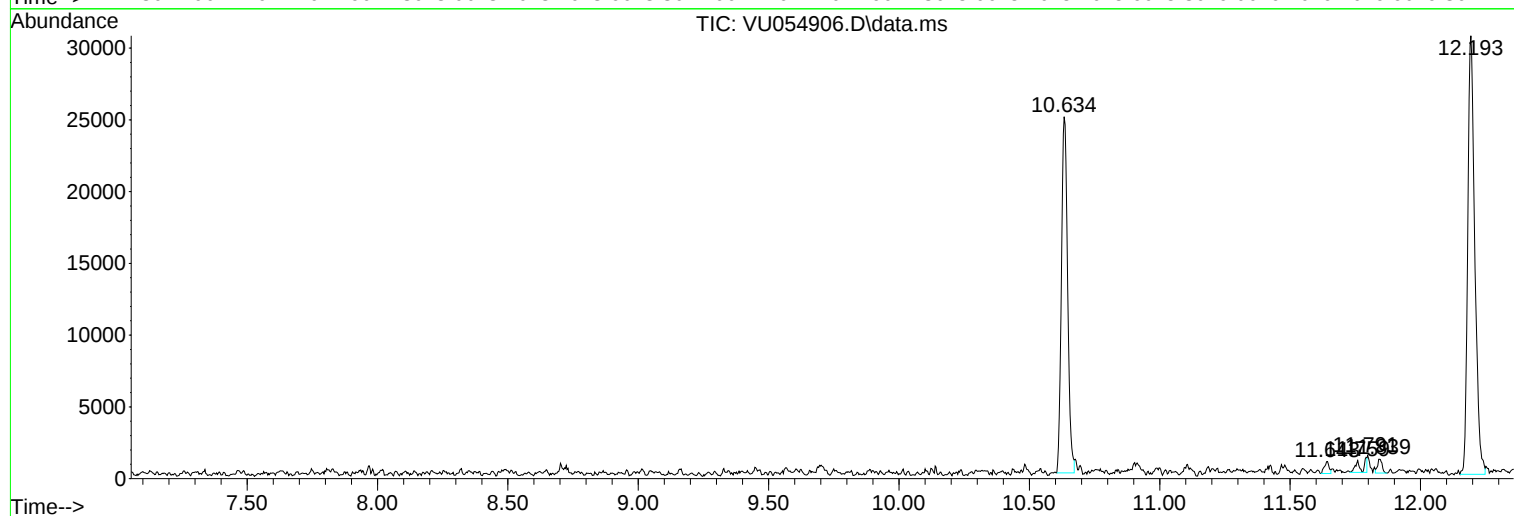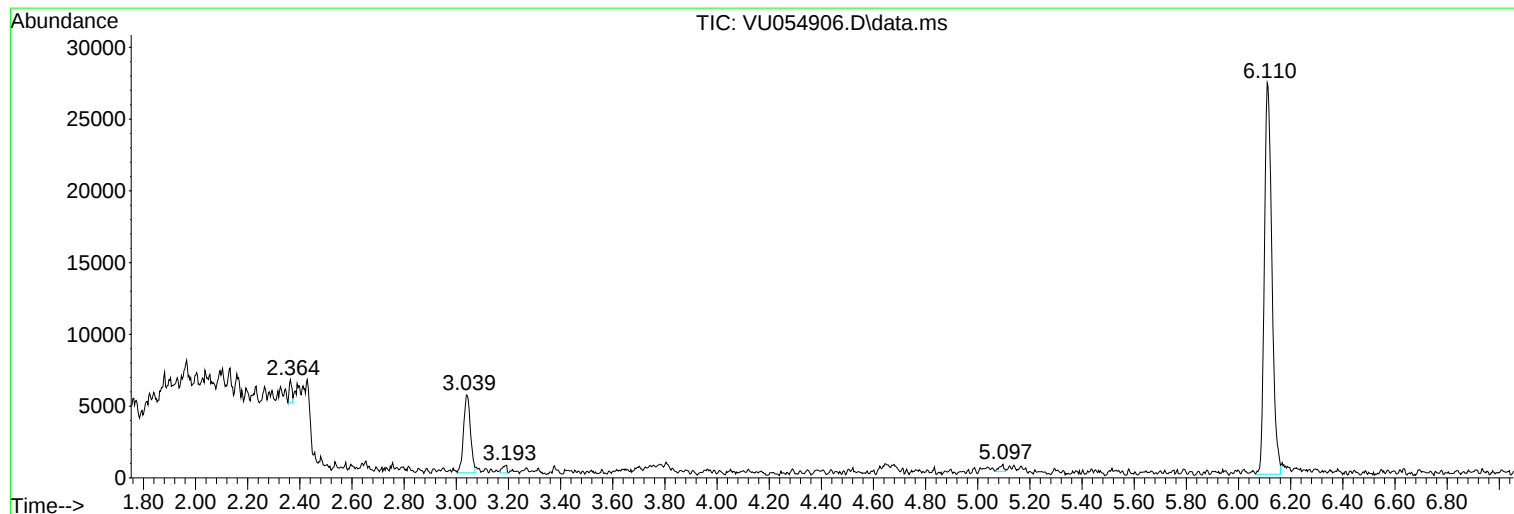

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
Data File : VU054906.D
Acq On : 28 Jul 2023 11:17
Operator : MD/SY
Sample : VU0728WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0728WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072823\
Data File : VU054906.D
Acq On : 28 Jul 2023 11:17
Operator : MD/SY
Sample : VU0728WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0728WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------