


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072919\
 Data File : VU033466.D
 Acq On : 29 Jul 2019 09:07
 Operator : JC/SP
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM072919W.M
 Title : VOC Analysis
 Last Update : Tue Jul 30 04:12:14 2019

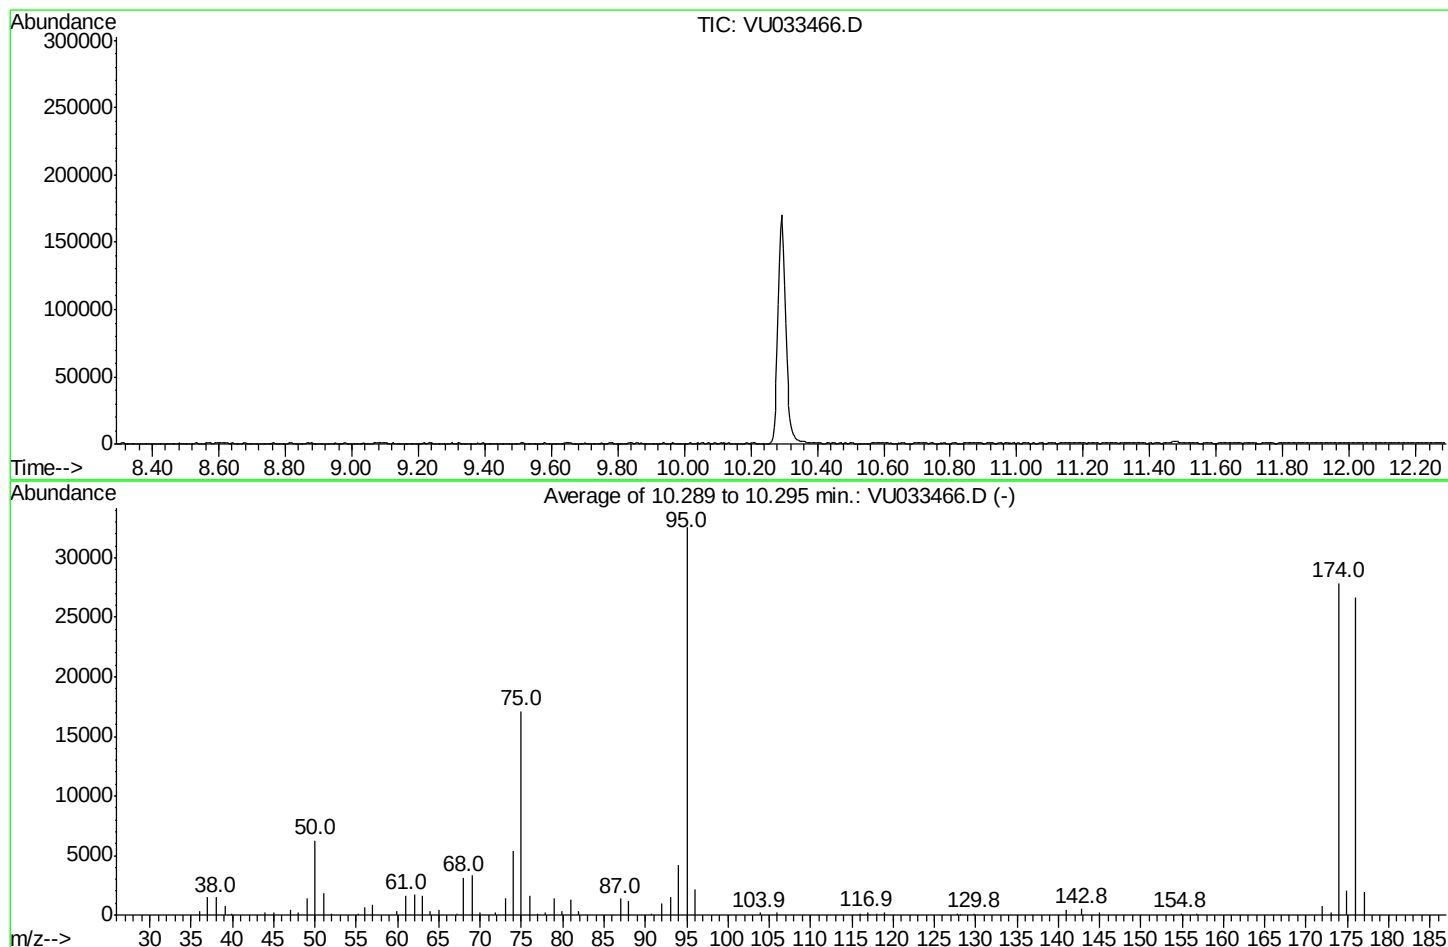

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6283	PASS
75	95	30	80	52.7	17144	PASS
95	95	100	100	100.0	32560	PASS
96	95	5	9	6.5	2111	PASS
173	174	0.00	2	0.6	176	PASS
174	95	50	120	85.6	27864	PASS
175	174	5	9	7.5	2099	PASS
176	174	95	101	95.7	26674	PASS
177	176	5	9	7.4	1963	PASS

Scan 2850 (10.254 min): VU033466.D
BFB40

m/z	Abundance
39.90	121.0
43.90	361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	307.0
37.00	1444.0
38.00	1397.0
39.10	833.0
39.90	206.0
44.00	608.0
44.90	263.0
47.00	429.0
47.90	194.0
49.00	1418.0
50.00	6294.0
51.00	1812.0
51.90	123.0
55.20	132.0
56.10	565.0
57.00	861.0
59.90	313.0
61.00	1537.0
62.00	1730.0
63.10	1662.0
63.90	341.0
65.00	433.0
67.10	130.0
68.00	3127.0
69.00	3229.0
70.00	214.0
71.90	213.0
73.00	1317.0
74.00	5101.0
75.00	16616.0
76.00	1538.0
77.00	157.0
77.90	256.0
78.90	1347.0
79.90	293.0
80.90	1319.0
81.90	246.0
87.00	1393.0
88.00	1162.0
90.80	127.0
91.90	917.0
93.00	1412.0
94.00	3965.0
95.00	31992.0
96.00	2159.0
103.90	190.0
105.90	189.0
115.90	107.0
116.90	238.0
118.00	114.0
118.90	227.0
128.10	101.0
129.80	118.0
140.90	452.0
142.80	430.0
145.00	241.0
154.90	146.0
156.80	107.0
172.00	591.0
174.00	26360.0
174.90	2070.0
176.00	25176.0
177.00	1922.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	329.0
37.00	1517.0
38.00	1546.0
39.10	797.0
40.00	187.0
44.00	607.0
44.90	257.0
47.00	483.0
48.00	212.0
49.00	1497.0
50.00	6521.0
51.00	1883.0
52.00	108.0
55.20	117.0
56.00	621.0
57.00	890.0
60.00	315.0
61.00	1706.0
62.00	1756.0
63.00	1681.0
63.90	340.0
65.00	443.0
67.10	117.0
68.00	3228.0
69.00	3386.0
69.90	251.0
71.90	202.0
73.00	1485.0
74.00	5583.0
75.00	17768.0
76.00	1593.0
77.00	161.0
77.90	198.0
78.90	1508.0
79.90	328.0
80.90	1345.0
81.90	295.0
87.00	1433.0
88.00	1173.0
90.80	144.0
91.90	1054.0
93.00	1540.0
94.00	4404.0
95.00	33640.0
96.00	2215.0
103.90	185.0
105.90	190.0
115.90	118.0
116.90	248.0
118.00	107.0
119.00	208.0
127.80	105.0
129.90	142.0
140.90	432.0
142.80	517.0
145.00	190.0
154.90	127.0
156.80	105.0
172.00	736.0
174.00	28840.0
174.90	2176.0
176.00	27544.0
177.00	2052.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	317.0
37.00	1442.0
38.00	1556.0
39.10	658.0
40.00	169.0
44.00	546.0
45.00	228.0
47.00	461.0
48.00	206.0
49.00	1433.0
50.00	6034.0
51.00	1813.0
52.00	101.0
56.00	625.0
57.00	907.0
60.00	302.0
61.00	1691.0
62.00	1625.0
63.00	1552.0
63.90	283.0
65.00	425.0
68.00	3088.0
69.00	3266.0
69.90	247.0
71.90	186.0
73.00	1485.0
74.00	5503.0
75.00	17048.0
76.00	1562.0
77.00	159.0
77.90	120.0
78.90	1416.0
79.90	311.0
80.90	1277.0
81.90	345.0
87.00	1359.0
88.00	1130.0
90.80	141.0
92.00	1083.0
93.00	1518.0
94.00	4265.0
95.00	32048.0
96.00	1961.0
103.90	197.0
105.90	175.0
116.00	108.0
116.90	241.0
118.80	196.0
127.80	102.0
129.90	134.0
140.90	368.0
142.90	568.0
144.90	126.0
154.80	111.0
171.90	853.0
173.00	530.0
174.00	28392.0
174.90	2051.0
176.00	27304.0
177.00	1917.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40