

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072920\
 Data File : VU039708.D
 Acq On : 29 Jul 2020 17:24
 Operator : SY/MD
 Sample : L3319-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01

Quant Time: Jul 31 14:02:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 31 07:12:27 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	6.13	96	20413	1.00	ug/l	0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.63	95	7774	0.97	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.00%	
68) 1,2-Dichlorobenzene-d4	12.19	152	8148	1.04	ug/l	0.00
Spiked Amount 1.000			Recovery	=	104.00%	
Target Compounds					Ovalue	
3) Chloromethane	1.53	50	168686	19.144	ug/l	100
6) Chloroethane	1.94	64	90172	16.004	ug/l	99
17) 1,1-Dichloroethane	3.89	63	105847	7.475	ug/l	99
21) 2,2-Dichloropropane	4.68	77	172815	14.961	ug/l	96
25) Methyl tert-Butyl Ether	3.38	73	626186	33.836	ug/l	98
26) Bromochloromethane	4.99	128	43480	15.290	ug/l	100
29) 1,1-Dichloropropene	5.54	75	40866	3.958	ug/l	98
43) Dibromomethane	6.93	93	29319	7.740	ug/l	99
50) t-1,3-Dichloropropene	8.22	75	128220	16.391	ug/l	99
51) cis-1,3-Dichloropropene	7.62	75	137354	14.939	ug/l	98
53) 1,3-Dichloropropane	8.58	76	121629	12.870	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.54	131	67732	12.778	ug/l	98
69) Isopropylbenzene	10.48	105	275926	9.885	ug/l	100
70) 1,1,2,2-Tetrachloroethane	10.78	83	129984	18.346	ug/l	97
71) 1,2,3-Trichloropropane	10.83	75	94468	17.699	ug/l	87
72) Bromobenzene	10.78	156	42764	6.746	ug/l	98
73) n-propylbenzene	10.91	120	105506	13.443	ug/l	95
74) 2-Chlorotoluene	10.99	126	50997	7.691	ug/l	98
75) 1,3,5-Trimethylbenzene	11.09	105	432104	17.906	ug/l	100
76) 4-Chlorotoluene	11.10	126	68148	9.923	ug/l	84
77) tert-Butylbenzene	11.42	119	236030	10.196	ug/l	92
78) 1,2,4-Trimethylbenzene	11.46	105	468641	18.936	ug/l	99
79) sec-Butylbenzene	11.64	105	299999	9.104	ug/l	100
81) p-Isopropyltoluene	11.79	119	464907	17.507	ug/l	100
82) 1,3-Dichlorobenzene	11.74	146	206277	15.118	ug/l	99
84) n-Butylbenzene	12.20	91	187014	6.630	ug/l	100
88) Hexachlorobutadiene	14.01	225	53045	14.201	ug/l	97
89) Naphthalene	14.08	128	887100	50.405	ug/l	99
90) 1,2,3-Trichlorobenzene	14.32	180	298762	38.476	ug/l	99
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072920\
Data File : VU039708.D
Acq On : 29 Jul 2020 17:24
Operator : SY/MD
Sample : L3319-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0729WBS01

Quant Time: Jul 31 14:02:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 31 07:12:27 2020
Response via : Initial Calibration

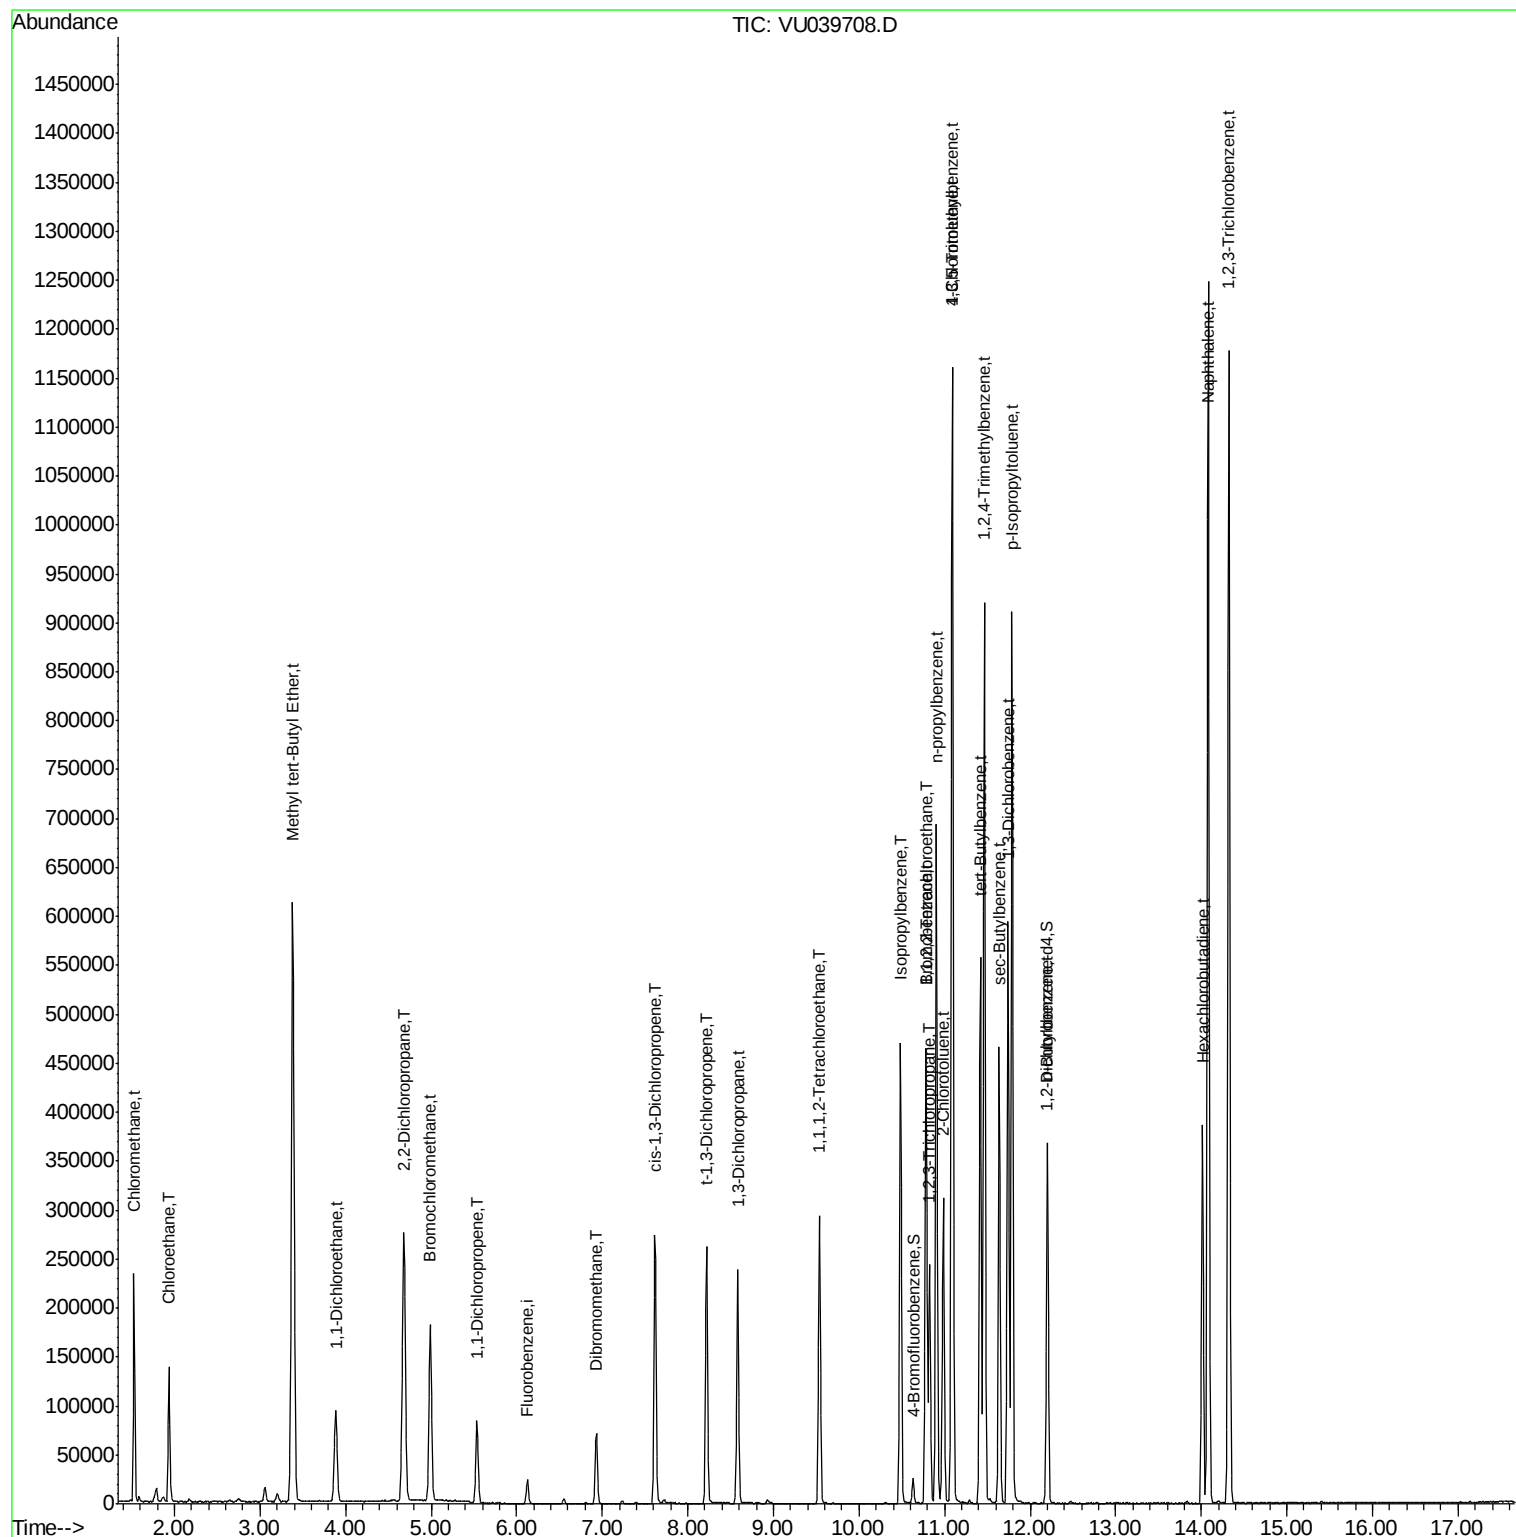



#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.13 min Scan# 1489

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24

Instrument :

MSVOA_U

ClientSampleId :

VU0729WBS01

Tot Ion: 96 Resp: 20413


Ion Ratio Lower Upper

96 100

70 20.9 16.3 24.5

95 9.6 6.8 10.2

97 6.3 0.0 0.0#



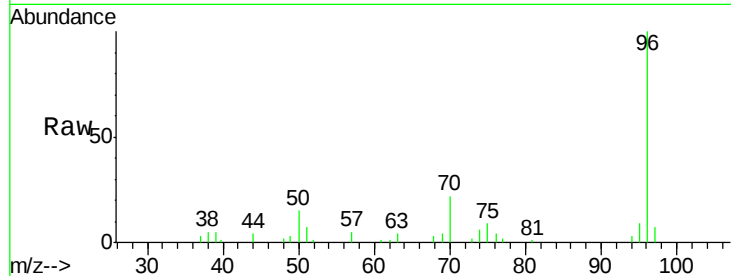


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

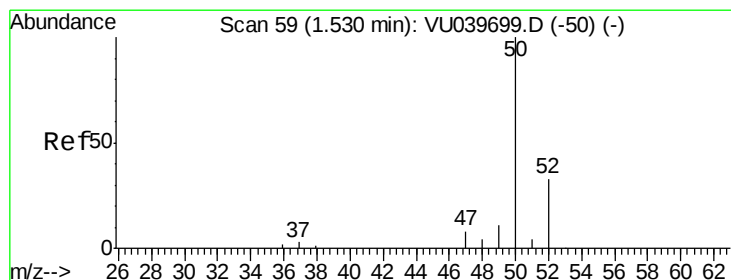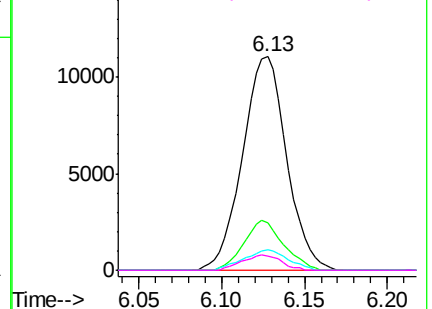

#3

Chloromethane

Concen: 19.144 ug/l

RT: 1.53 min Scan# 59

Delta R.T. -0.00 min

Lab File: VU039708.D


Acq: 29 Jul 2020 17:24

Tgt Ion: 50 Resp: 168686

Ion Ratio Lower Upper



50 100


52 32.6 26.0 39.0

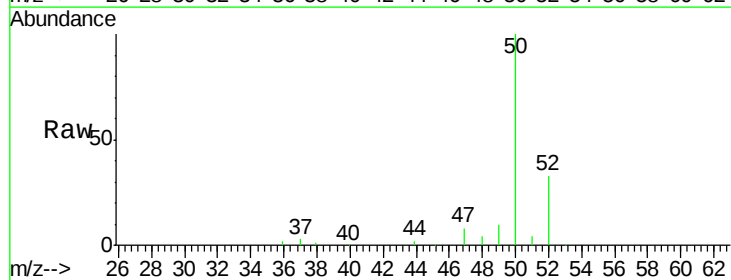

Abundance Ion 50.00 (49.70 to 50.70): VU0

Ion 52.00 (51.70 to 52.70): VU0



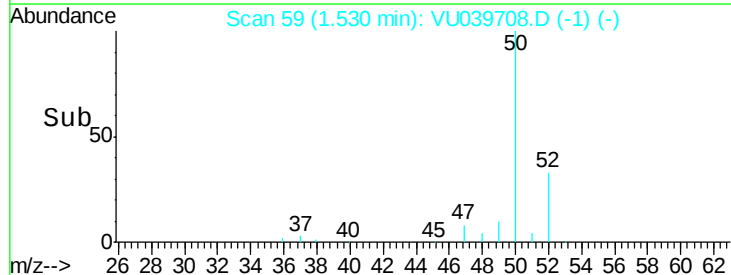
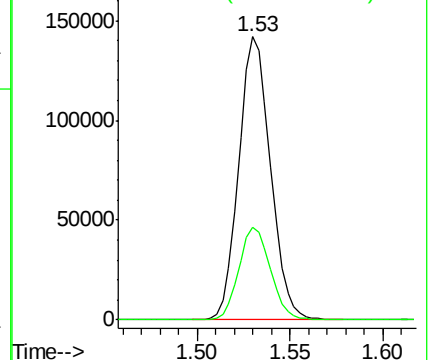


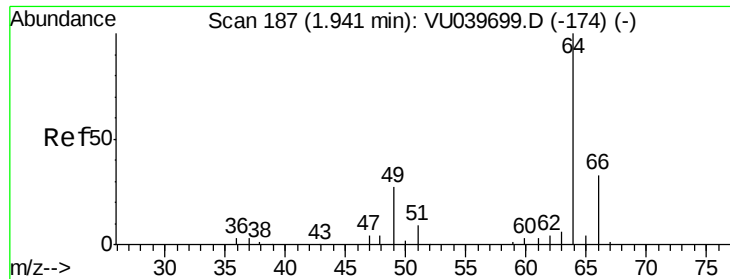

#6
 Chloroethane
 Concen: 16.004 ug/l
 RT: 1.94 min Scan# 186
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion: 64 Resp: 90172
 Ion Ratio Lower Upper
 64 100
 66 32.2 26.2 39.2

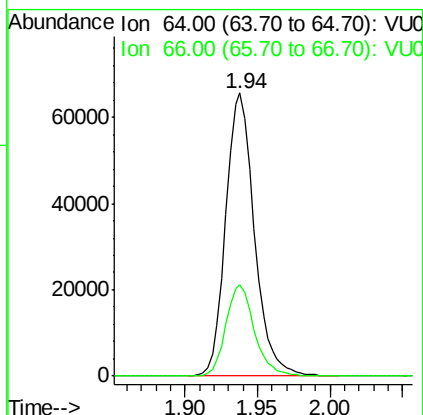

#17
 1,1-Dichloroethane
 Concen: 7.475 ug/l
 RT: 3.89 min Scan# 792
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion: 63 Resp: 105847
 Ion Ratio Lower Upper
 63 100
 98 5.6 2.9 8.7
 100 3.4 2.0 6.0



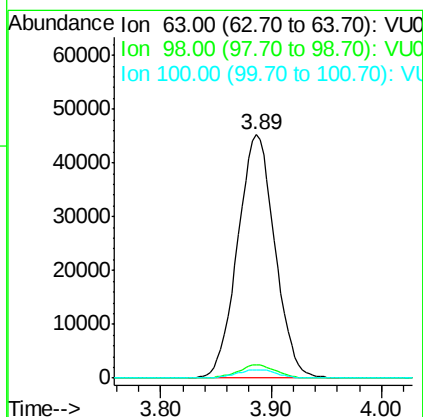





#21
 2,2-Dichloropropane
 Concen: 14.961 ug/l
 RT: 4.68 min Scan# 1039
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion: 77 Resp: 172815
 Ion Ratio Lower Upper
 77 100
 97 17.4 15.2 22.8

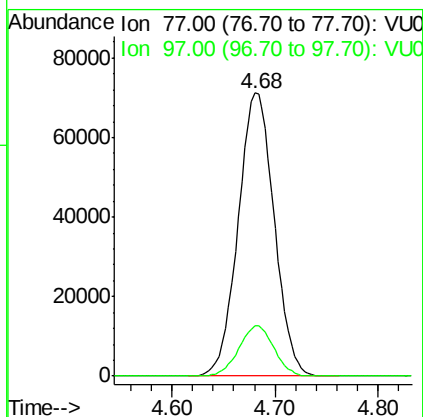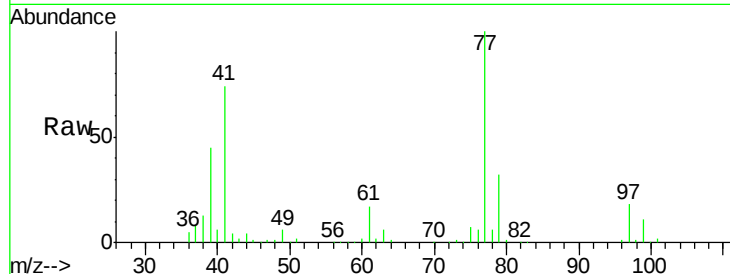

#25
 Methyl tert-Butyl Ether
 Concen: 33.836 ug/l
 RT: 3.38 min Scan# 636
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion: 73 Resp: 626186
 Ion Ratio Lower Upper
 73 100
 43 24.2 20.1 30.1

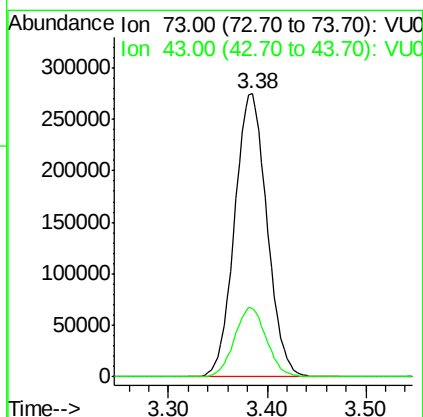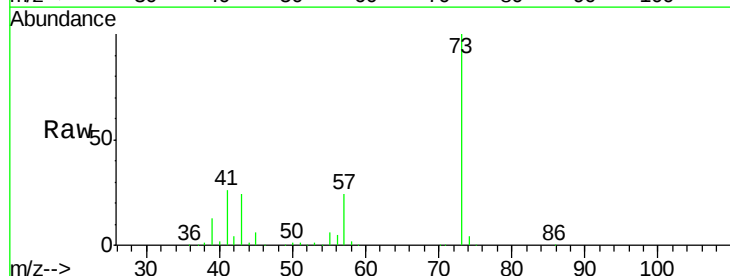







#26
 Bromochloromethane
 Concen: 15.290 ug/l
 RT: 4.99 min Scan# 1136
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01

Tot Ion:128 Resp: 43480
 Ion Ratio Lower Upper
 128 100
 49 251.0 0.0 503.8
 130 128.7 102.7 154.1

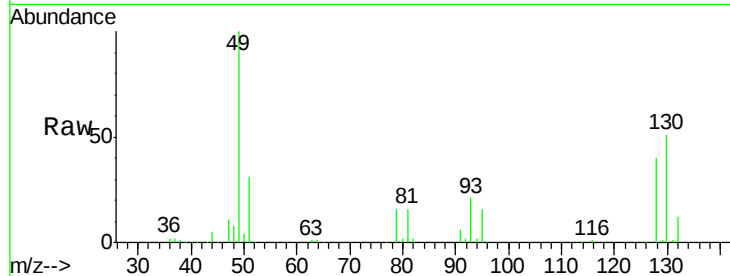


Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 49.00 (48.70 to 49.70): VU0
 Ion 130.00 (129.70 to 130.70): V


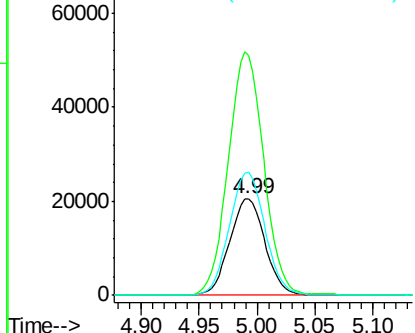



#29
 1,1-Dichloropropene
 Concen: 3.958 ug/l
 RT: 5.54 min Scan# 1305
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion: 75 Resp: 40866
 Ion Ratio Lower Upper
 75 100
 110 31.2 14.6 44.0
 77 31.6 25.0 37.4



Abundance Ion 75.00 (74.70 to 75.70): VU0
 Ion 110.00 (109.70 to 110.70): V
 Ion 77.00 (76.70 to 77.70): VU0

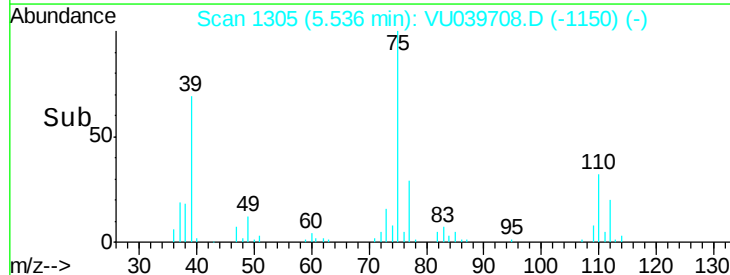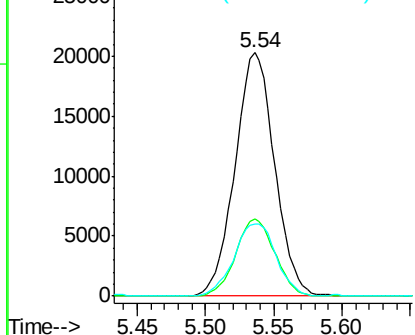



#43

Dibromomethane

Concen: 7.740 ug/l

RT: 6.93 min Scan# 1738

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24

Instrument :

MSVOA_U

ClientSampleId :

VU0729WBS01


Tot Ion: 93 Resp: 29319

Ion Ratio Lower Upper

93 100

95 81.8 66.6 99.8

174 78.6 62.7 94.1

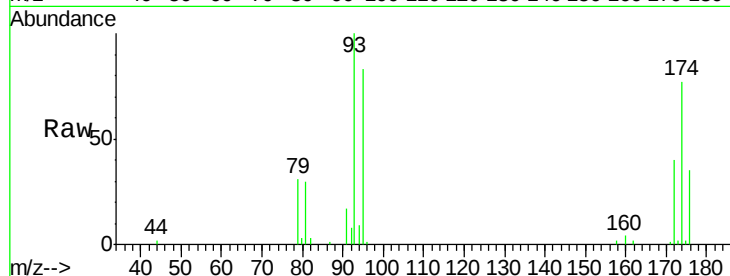


Abundance Ion 93.00 (92.70 to 93.70): VU039699.D (-1726) (-)

Ion 95.00 (94.70 to 95.70): VU039699.D (-1726) (-)

Ion 174.00 (173.70 to 174.70): VU039699.D (-1726) (-)

Time-->




Abundance Ion 93.00 (92.70 to 93.70): VU039708.D (-1584) (-)

Ion 95.00 (94.70 to 95.70): VU039708.D (-1584) (-)

Ion 174.00 (173.70 to 174.70): VU039708.D (-1584) (-)

Time-->



#50

t-1,3-Dichloropropene

Concen: 16.391 ug/l

RT: 8.22 min Scan# 2140

Delta R.T. -0.00 min

Lab File: VU039708.D


Acq: 29 Jul 2020 17:24

Tgt Ion: 75 Resp: 128220

Ion Ratio Lower Upper

75 100


77 30.9 24.3 36.5



Abundance Ion 75.00 (74.70 to 75.70): VU039699.D (-2126) (-)

Ion 77.00 (76.70 to 77.70): VU039699.D (-2126) (-)


Time-->



Abundance Ion 75.00 (74.70 to 75.70): VU039708.D (-1985) (-)

Ion 77.00 (76.70 to 77.70): VU039708.D (-1985) (-)

Time-->







#51

cis-1,3-Dichloropropene
 Concen: 14.939 ug/l
 RT: 7.62 min Scan# 1953
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01




Tot Ion: 75 Resp: 137354
 Ion Ratio Lower Upper
 75 100
 77 31.5 25.7 38.5
 39 59.5 46.1 69.1

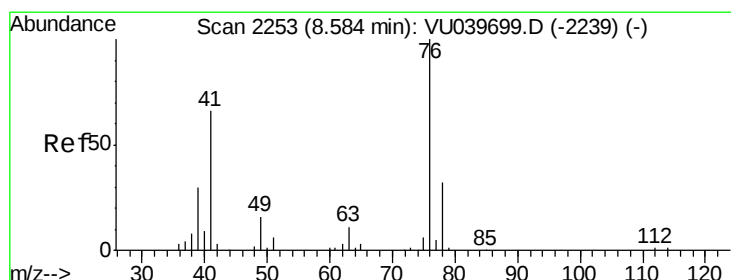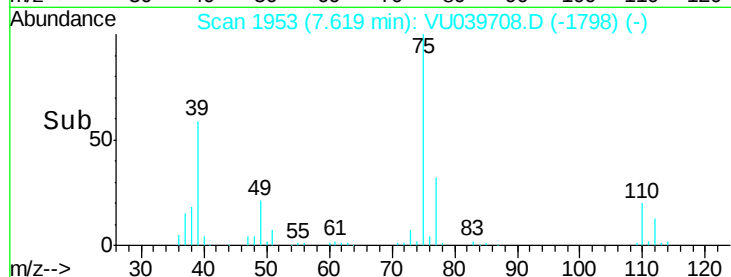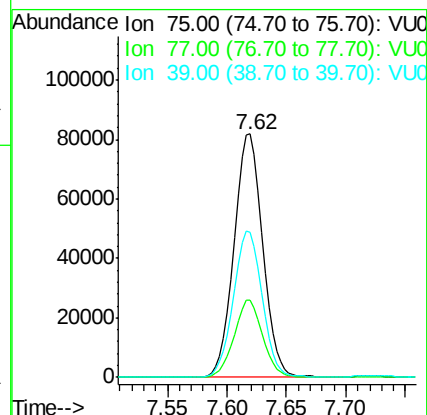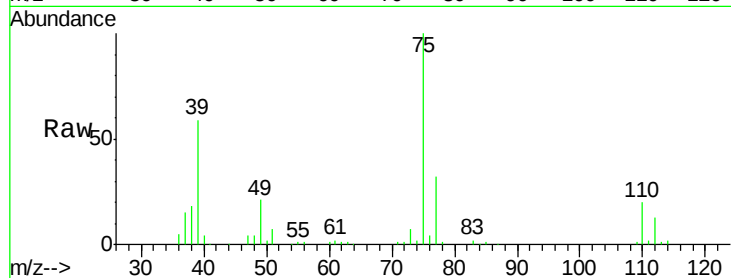


#53

1,3-Dichloropropane
 Concen: 12.870 ug/l
 RT: 8.58 min Scan# 2253
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion: 76 Resp: 121629
 Ion Ratio Lower Upper
 76 100
 78 32.2 25.4 38.2

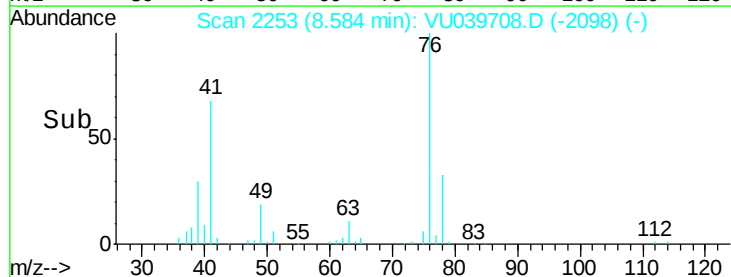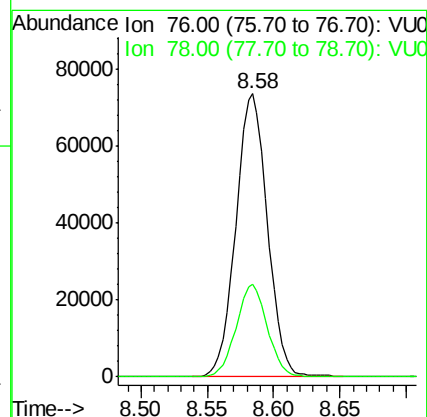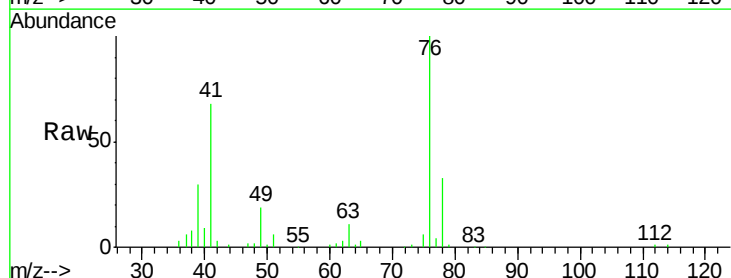

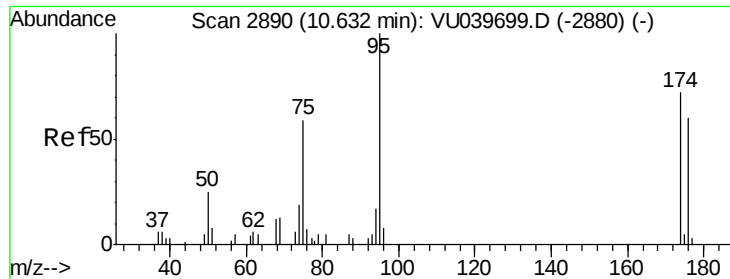

#57

4-Bromofluorobenzene

Concen: 0.974 ug/l

RT: 10.63 min Scan# 2890

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24

Instrument :

MSVOA_U

ClientSampleId :

VU0729WBS01


Tot Ion: 95 Resp: 7774

Ion Ratio Lower Upper

95 100

174 72.0 57.0 85.4

176 69.2 50.2 75.2




Abundance Ion 95.00 (94.70 to 95.70): VU039699.D (-2880) (-)

Ion 174.00 (173.70 to 174.70): VU039699.D (-2880) (-)

Ion 176.00 (175.70 to 176.70): VU039699.D (-2880) (-)

Time-->




Abundance Ion 95.00 (94.70 to 95.70): VU039708.D (-2579) (-)

Ion 174.00 (173.70 to 174.70): VU039708.D (-2579) (-)

Ion 176.00 (175.70 to 176.70): VU039708.D (-2579) (-)

Time-->



#60

1,1,1,2-Tetrachloroethane

Concen: 12.778 ug/l

RT: 9.54 min Scan# 2550

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24


Tgt Ion: 131 Resp: 67732

Ion Ratio Lower Upper

131 100

133 96.9 75.8 113.8

119 67.7 54.6 81.8




Abundance Ion 131.00 (130.70 to 131.70): VU039699.D (-2537) (-)

Ion 133.00 (132.70 to 133.70): VU039699.D (-2537) (-)

Ion 119.00 (118.70 to 119.70): VU039699.D (-2537) (-)

Time-->




Abundance Ion 131.00 (130.70 to 131.70): VU039708.D (-2395) (-)

Ion 133.00 (132.70 to 133.70): VU039708.D (-2395) (-)

Ion 119.00 (118.70 to 119.70): VU039708.D (-2395) (-)





Time-->

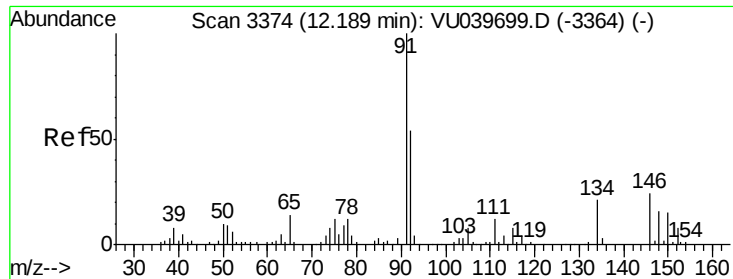

#68
 1,2-Dichlorobenzene-d4
 Concen: 1.044 ug/l
 RT: 12.19 min Scan# 3374
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion:152 Resp: 8148
 Ion Ratio Lower Upper
 152 100
 115 124.1 0.0 302.4
 150 160.0 0.0 645.8

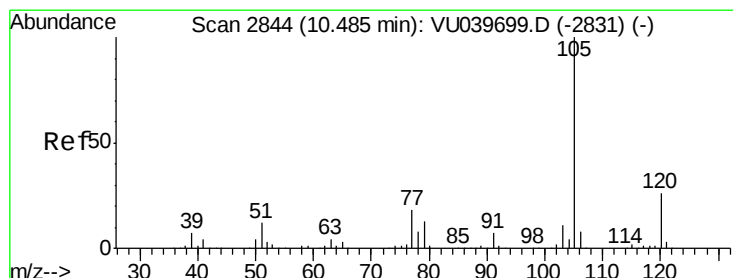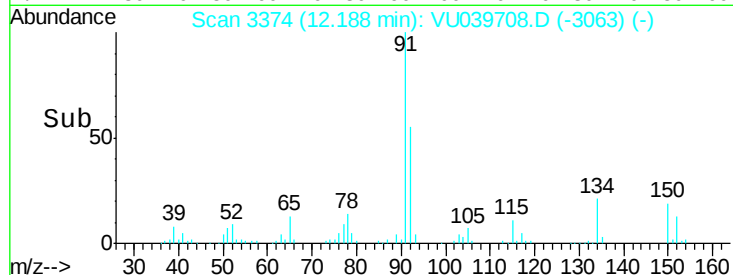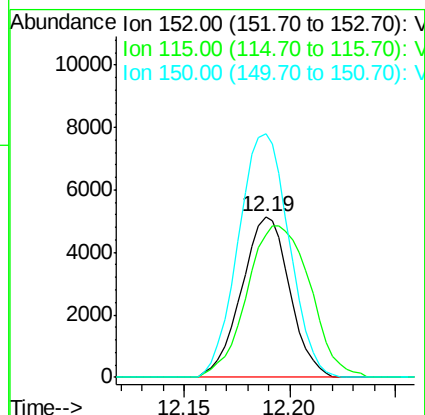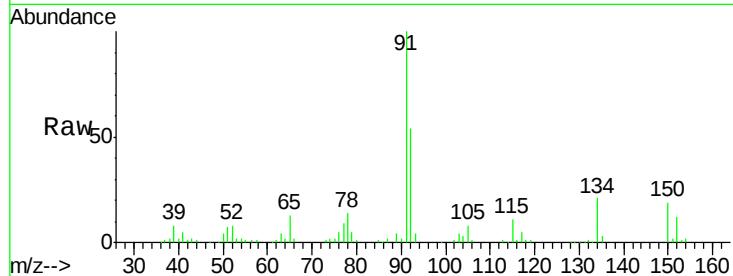

#69
 Isopropylbenzene
 Concen: 9.885 ug/l
 RT: 10.48 min Scan# 2844
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion:105 Resp: 275926
 Ion Ratio Lower Upper
 105 100
 120 25.4 12.8 38.4


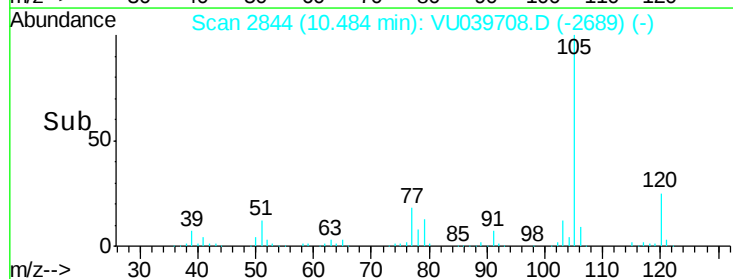
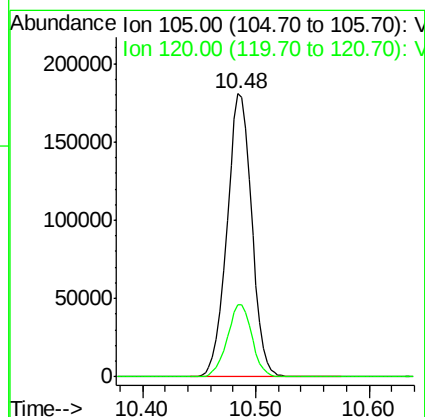
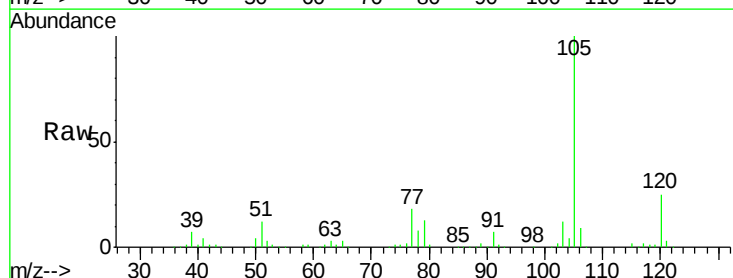




#70
 1,1,2,2-Tetrachloroethane
 Concen: 18.346 ug/l
 RT: 10.78 min Scan# 2937
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion: 83 Resp: 129984
 Ion Ratio Lower Upper
 83 100
 131 8.1 7.0 10.6
 85 65.4 50.6 75.8

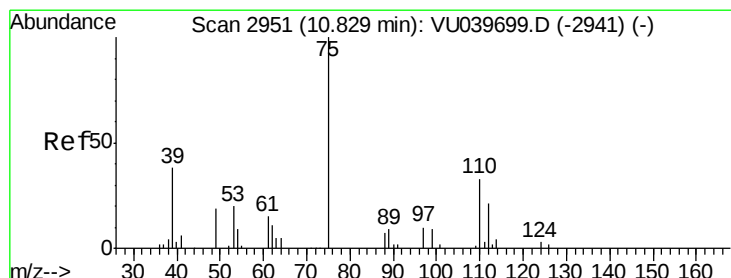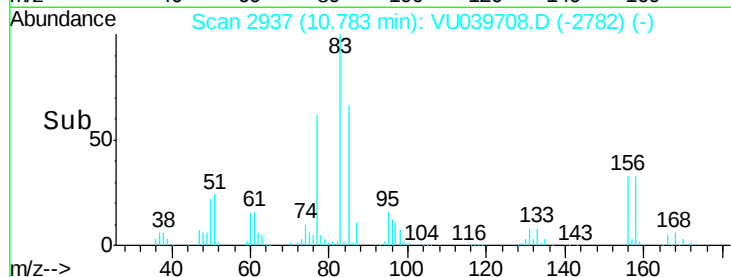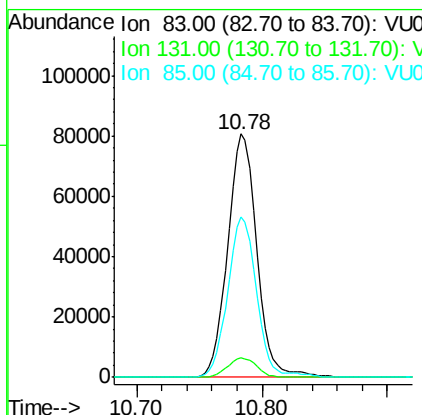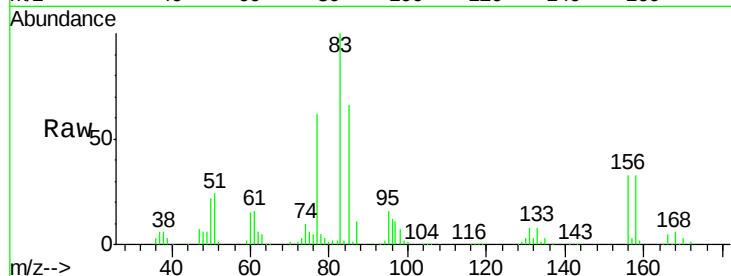

#71
 1,2,3-Trichloropropane
 Concen: 17.699 ug/l
 RT: 10.83 min Scan# 2950
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion: 75 Resp: 94468
 Ion Ratio Lower Upper
 75 100
 77 30.8 0.0 91.0
 110 35.5 0.0 64.2
 97 17.6 0.0 32.6

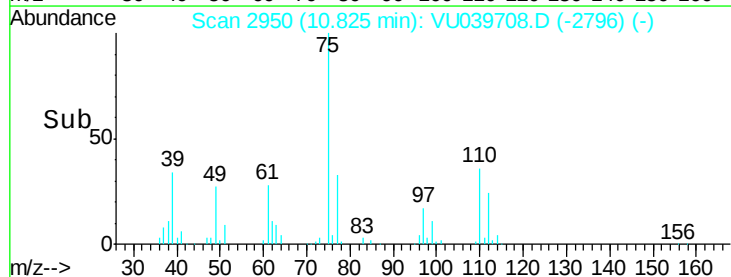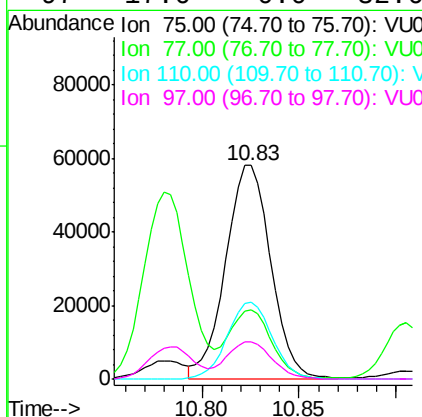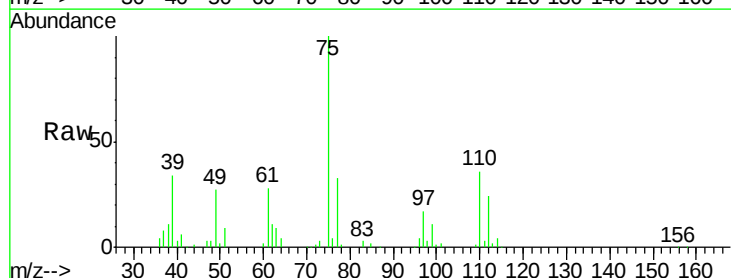



#72

Bromobenzene

Concen: 6.746 ug/l

RT: 10.78 min Scan# 2937

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24

Instrument :

MSVOA_U

ClientSampleId :

VU0729WBS01


Tot Ion:156 Resp: 42764

Ion Ratio Lower Upper

156 100

77 194.8 0.0 385.2




158 97.8 0.0 200.8

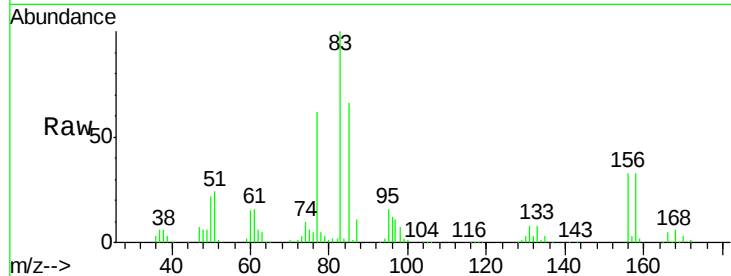

Abundance Ion 156.00 (155.70 to 156.70): V

Ion 77.00 (76.70 to 77.70): VU0

Ion 158.00 (157.70 to 158.70): V

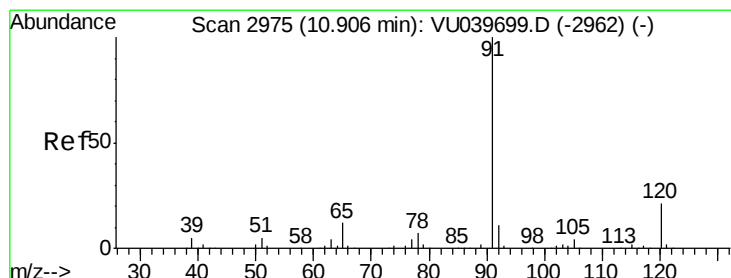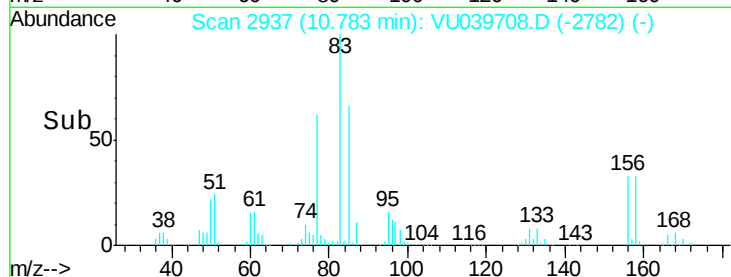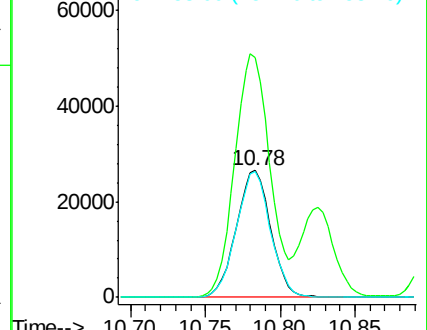

#73

n-propylbenzene

Concen: 13.443 ug/l

RT: 10.91 min Scan# 2975

Delta R.T. -0.00 min

Lab File: VU039708.D


Acq: 29 Jul 2020 17:24

Tgt Ion:120 Resp: 105506

Ion Ratio Lower Upper



120 100


91 476.7 371.7 557.5

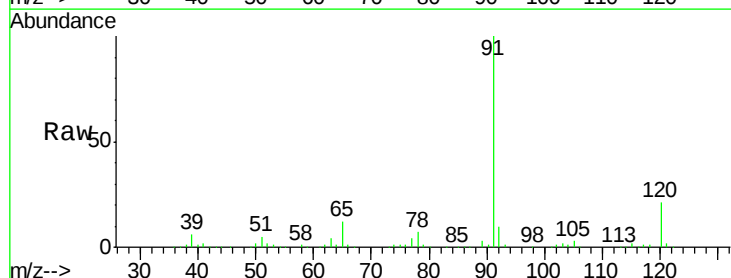

Abundance Ion 120.00 (119.70 to 120.70): V

Ion 91.00 (90.70 to 91.70): VU0

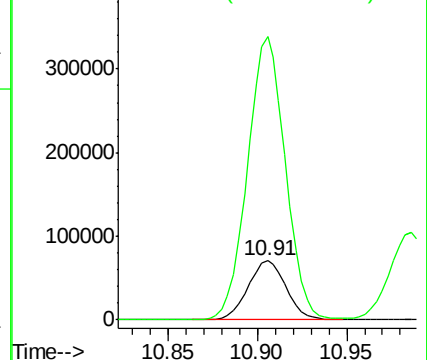

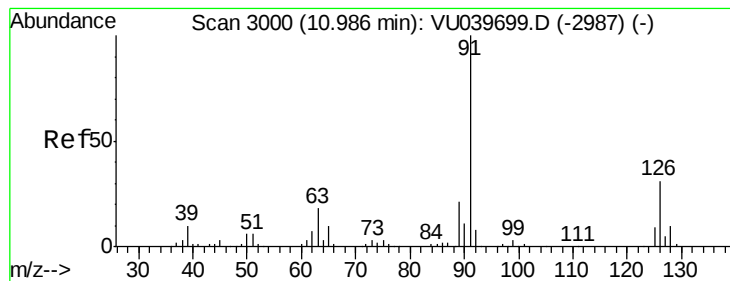

#74

2-Chlorotoluene

Concen: 7.691 ug/l

RT: 10.99 min Scan# 3000

Delta R.T. -0.00 min

Lab File: VU039708.D

Acq: 29 Jul 2020 17:24

Instrument :

MSVOA_U

ClientSampleId :


VU0729WBS01

Tot Ion:126 Resp: 50997

Ion Ratio Lower Upper




126 100

91 315.2 0.0 637.0



Abundance Ion 126.00 (125.70 to 126.70): V

Ion 91.00 (90.70 to 91.70): VU0

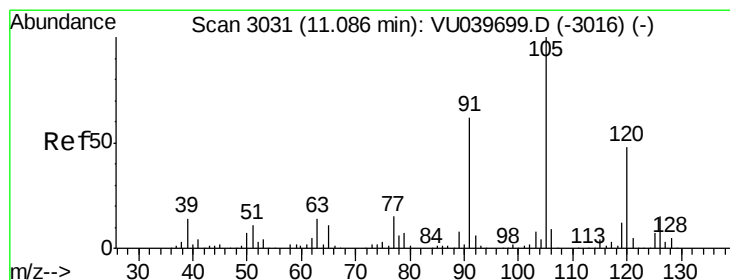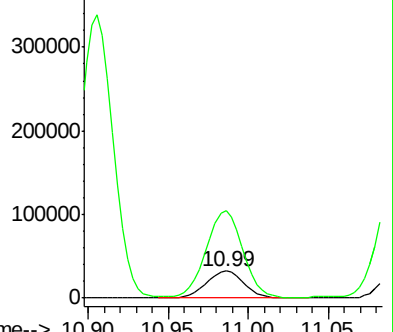

#75

1,3,5-Trimethylbenzene

Concen: 17.906 ug/l

RT: 11.09 min Scan# 3031

Delta R.T. -0.00 min

Lab File: VU039708.D


Acq: 29 Jul 2020 17:24

Tgt Ion:105 Resp: 432104

Ion Ratio Lower Upper



105 100


120 47.4 38.0 57.0



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V




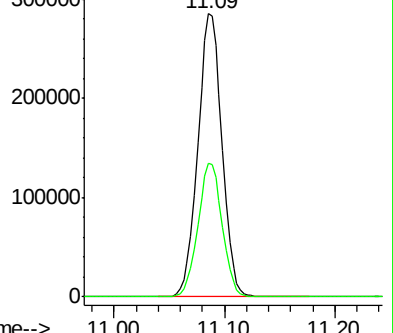




#76
4-Chlorotoluene
Concen: 9.923 ug/l
RT: 11.10 min Scan# 3034
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24




Instrument :
MSVOA_U
ClientSampleId :
VU0729WBS01


Tot Ion:126 Resp: 68148
Ion Ratio Lower Upper
126 100
91 401.5 0.0 732.2

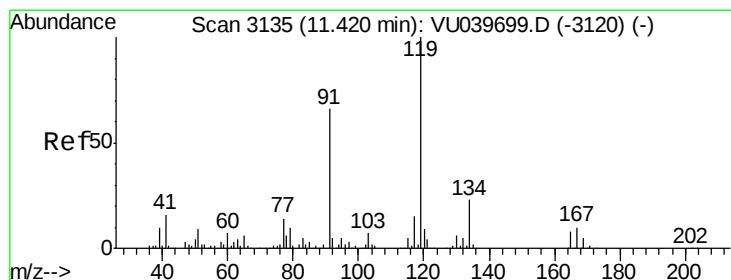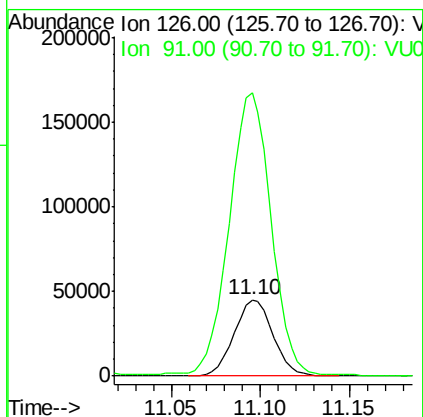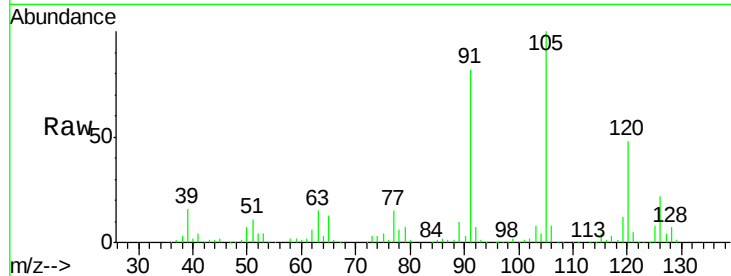

#77
tert-Butylbenzene
Concen: 10.196 ug/l
RT: 11.42 min Scan# 3134
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24

Tgt Ion:119 Resp: 236030
Ion Ratio Lower Upper
119 100
91 71.8 31.9 95.5
134 24.4 18.2 27.4


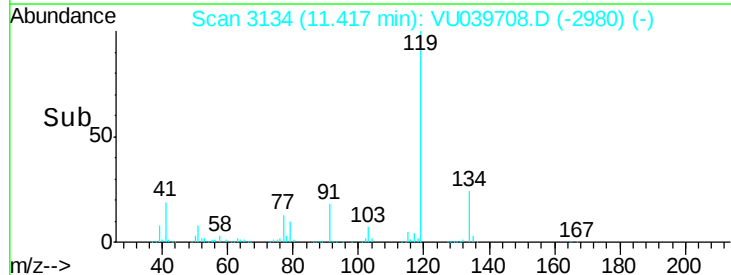
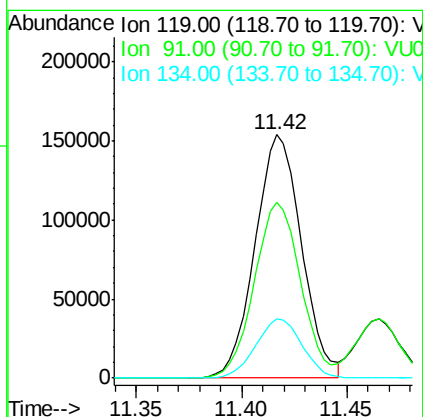
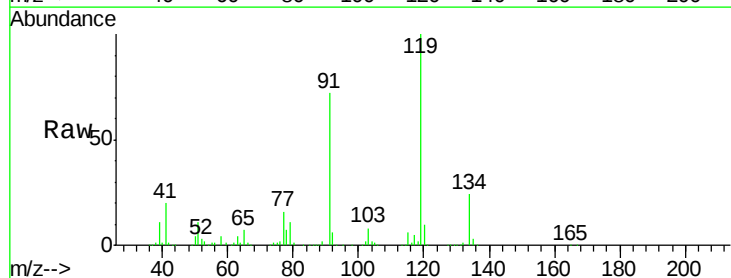


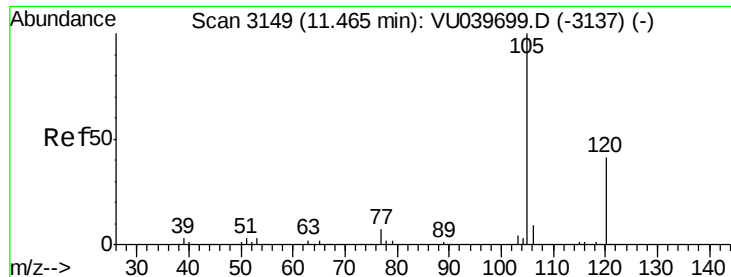

#78
 1,2,4-Trimethylbenzene
 Concen: 18.936 ug/l
 RT: 11.46 min Scan# 3149
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion:105 Resp: 468641
 Ion Ratio Lower Upper
 105 100
 120 44.9 22.7 68.0

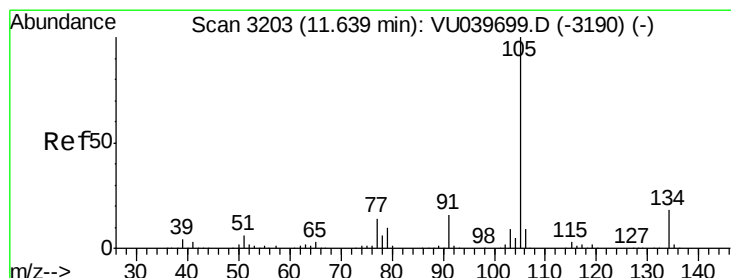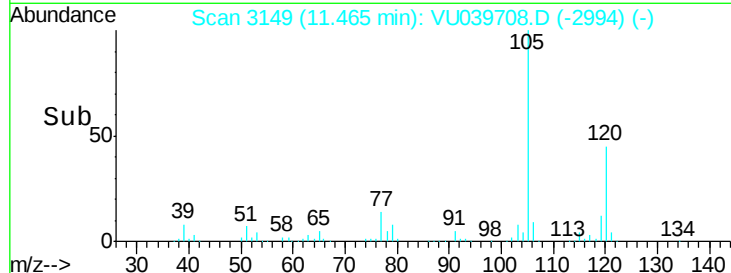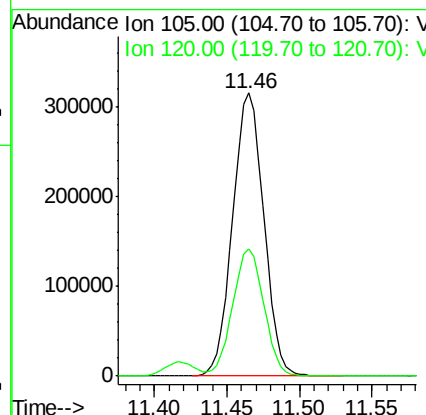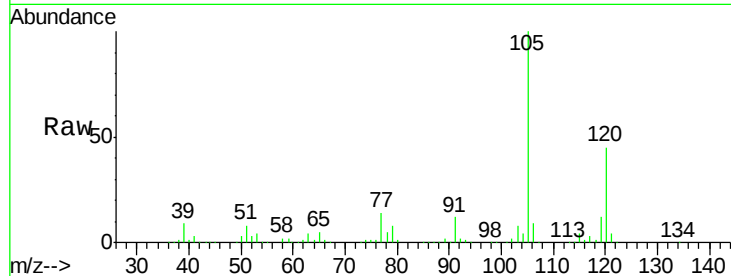

#79
 sec-Butylbenzene
 Concen: 9.104 ug/l
 RT: 11.64 min Scan# 3203
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion:105 Resp: 299999
 Ion Ratio Lower Upper
 105 100
 134 18.6 14.8 22.2


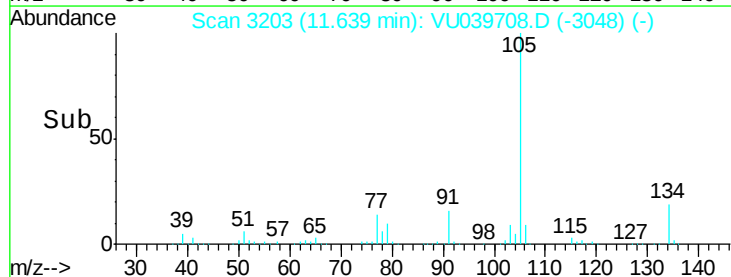
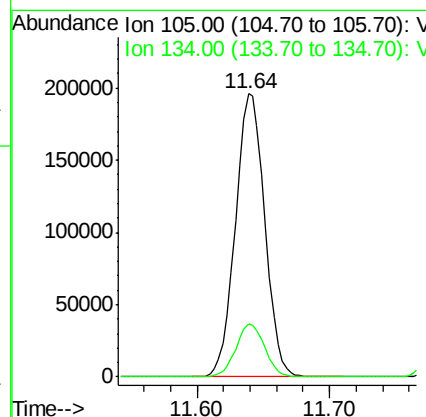
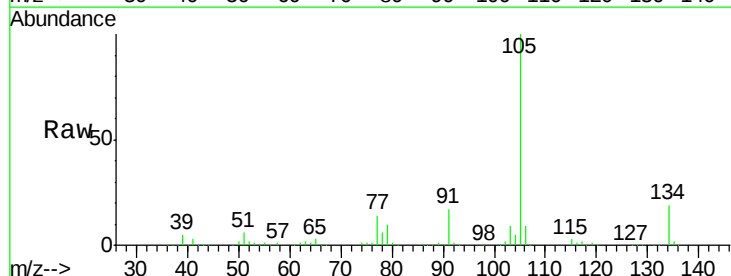


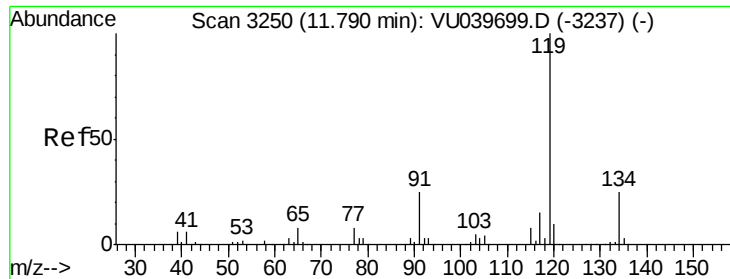

#81
 p-Isopropyltoluene
 Concen: 17.507 ug/l
 RT: 11.79 min Scan# 3250
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0729WBS01


Tot Ion	Ratio	Lower	Upper
119	100		
134	25.3	20.2	30.4
91	26.2	20.7	31.1

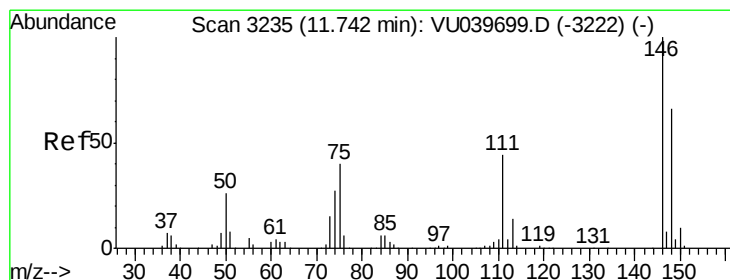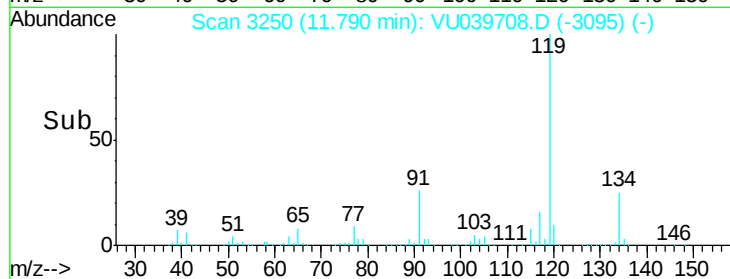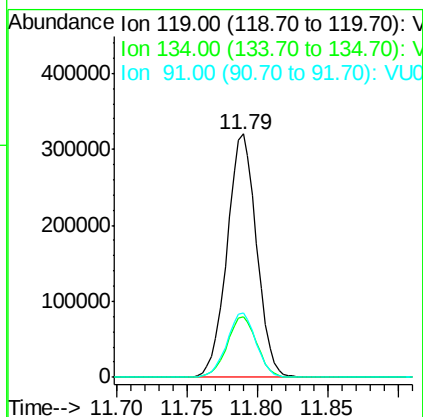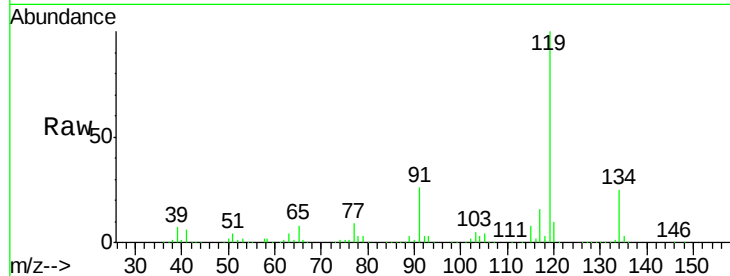

#82
 1,3-Dichlorobenzene
 Concen: 15.118 ug/l
 RT: 11.74 min Scan# 3235
 Delta R.T. -0.00 min
 Lab File: VU039708.D
 Acq: 29 Jul 2020 17:24

Tgt Ion	Ratio	Lower	Upper
146	100		
111	43.5	34.5	51.7
148	63.8	51.4	77.0


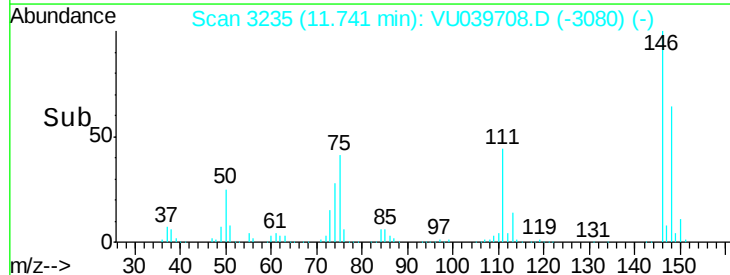
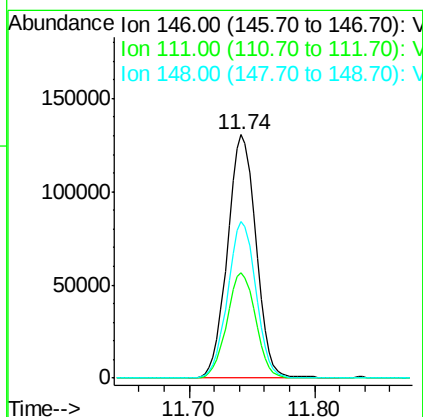



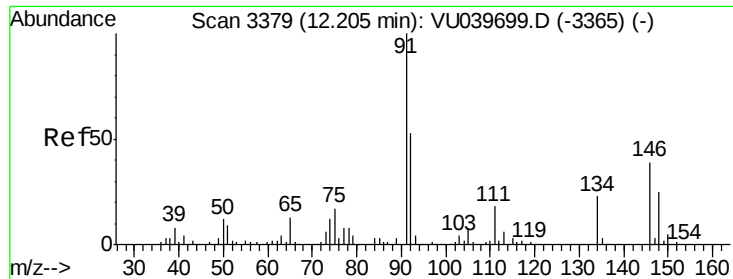

#84
n-Butylbenzene
Concen: 6.630 ug/l
RT: 12.20 min Scan# 3378
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24




Instrument :
MSVOA_U
ClientSampleId :
VU0729WBS01


Tot Ion: 91 Resp: 187014
Ion Ratio Lower Upper
91 100
92 53.3 42.6 64.0
134 23.1 18.2 27.4

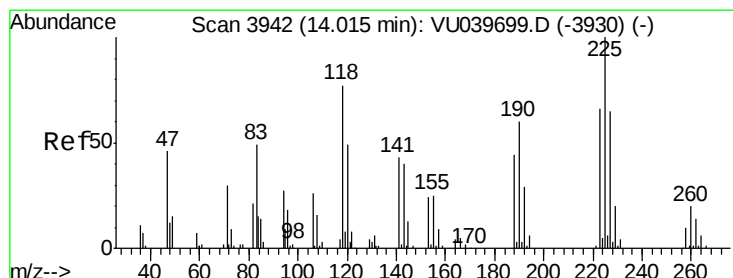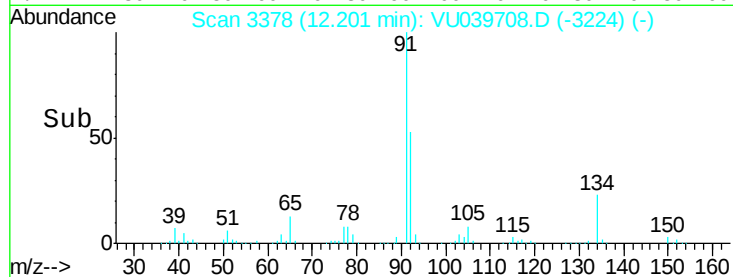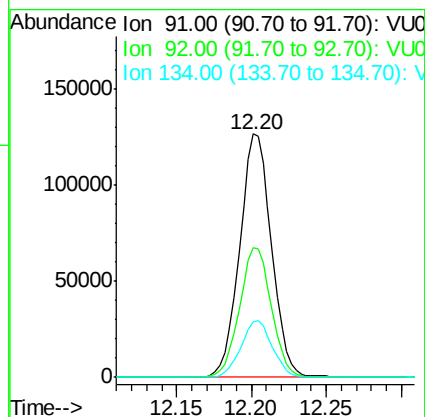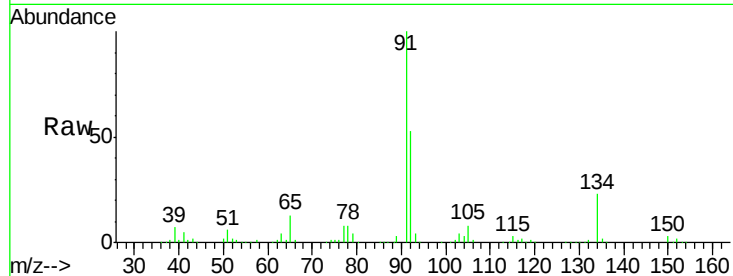

#88
Hexachlorobutadiene
Concen: 14.201 ug/l
RT: 14.01 min Scan# 3942
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24

Tgt Ion: 225 Resp: 53045
Ion Ratio Lower Upper
225 100
223 62.8 52.4 78.6
227 61.2 50.7 76.1


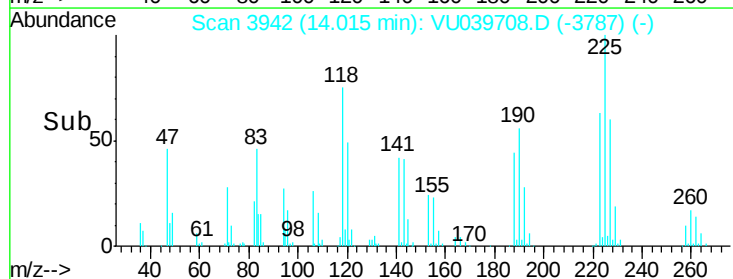
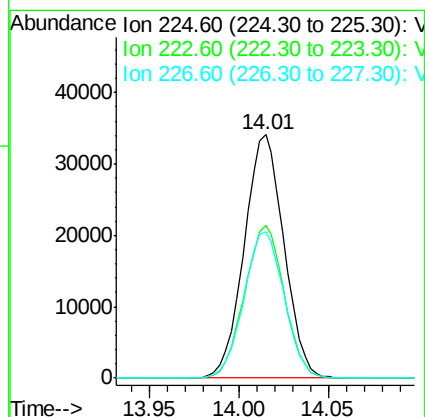
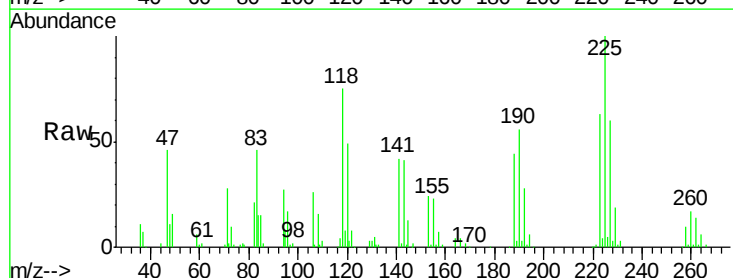




#89
Naphthalene
Concen: 50.405 ug/l
RT: 14.08 min Scan# 3962
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24

Instrument :
MSVOA_U
ClientSampleId :
VU0729WBS01

Tot Ion:128 Resp: 887100
Ion Ratio Lower Upper
128 100
127 13.9 11.0 16.4
129 10.8 8.4 12.6

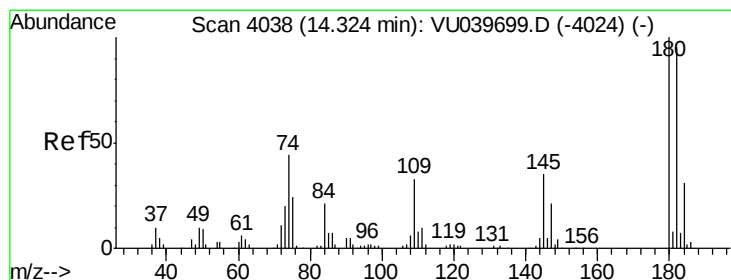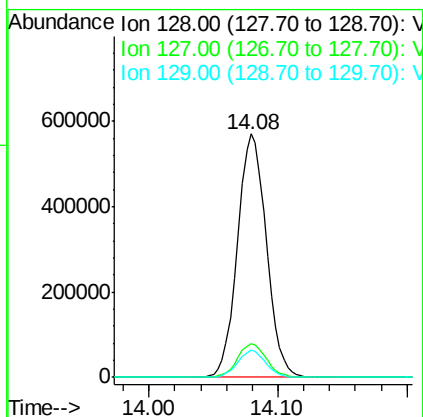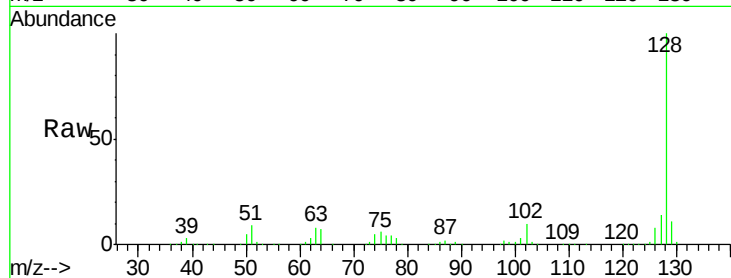

#90
1,2,3-Trichlorobenzene
Concen: 38.476 ug/l
RT: 14.32 min Scan# 4038
Delta R.T. -0.00 min
Lab File: VU039708.D
Acq: 29 Jul 2020 17:24

Tgt Ion:180 Resp: 298762
Ion Ratio Lower Upper
180 100
182 96.1 76.0 114.0
145 35.4 27.8 41.6

