

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072920\
Data File : VU039710.D
Acq On : 29 Jul 2020 18:24
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Jul 30 02:37:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 30 01:45:12 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	6.12	96	21240	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.63	95	6723	0.81	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.00%	
68) 1,2-Dichlorobenzene-d4	12.19	152	6625	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072920\
Data File : VU039710.D
Acq On : 29 Jul 2020 18:24
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Jul 30 02:37:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 30 01:45:12 2020
Response via : Initial Calibration

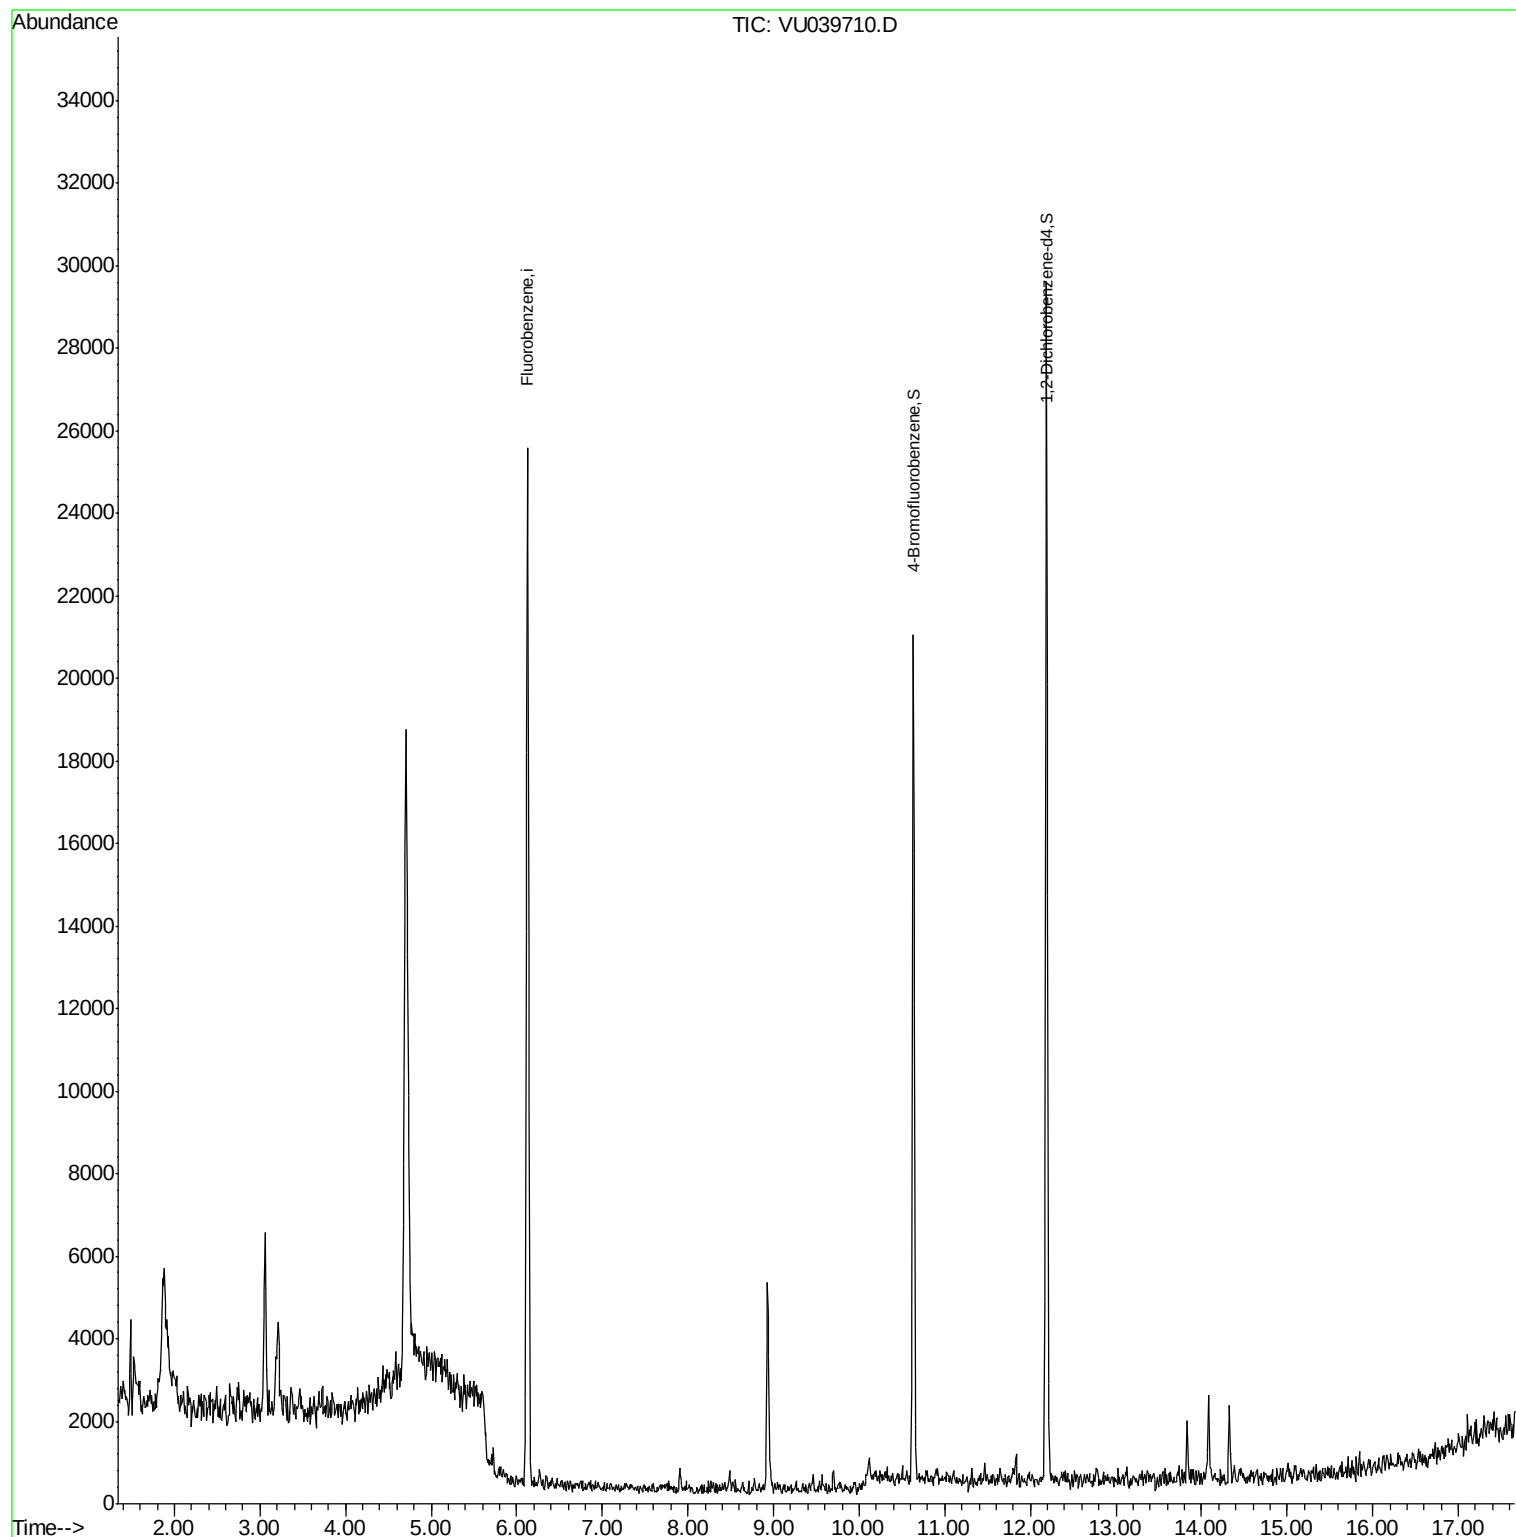

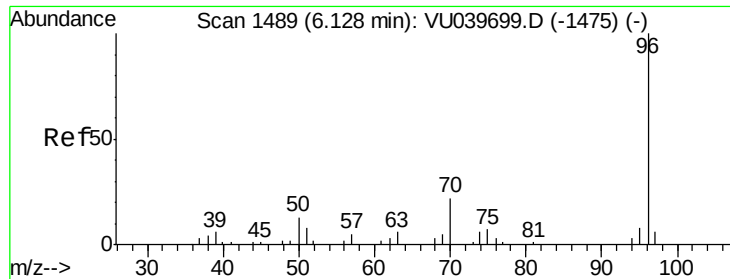

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.12 min Scan# 1488

Delta R.T. -0.00 min

Lab File: VU039710.D

Acq: 29 Jul 2020 18:24

Instrument :

MSVOA_U

ClientSampleId :

VIBLK

Tot Ion: 96 Resp: 21240


Ion Ratio Lower Upper

96 100

70 20.5 16.3 24.5

95 9.4 6.8 10.2

97 6.2 0.0 0.0#



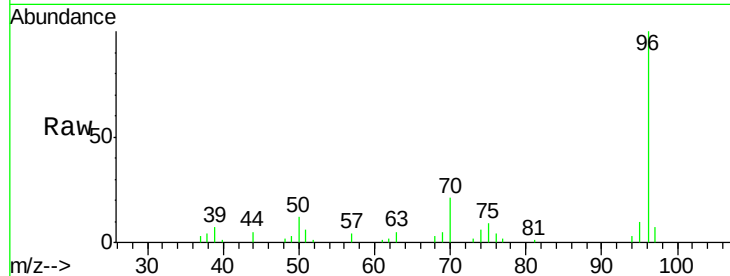


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

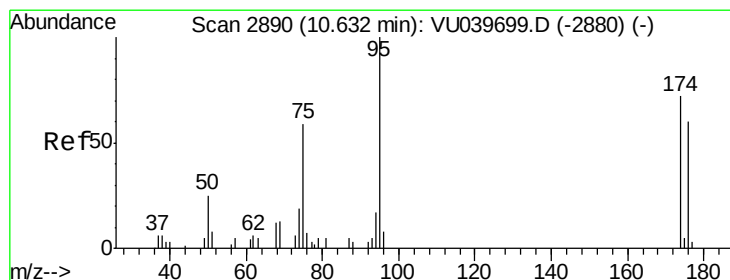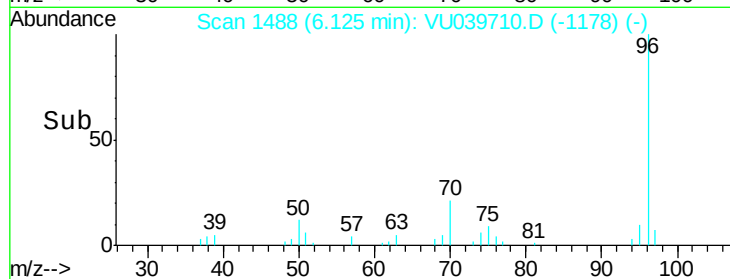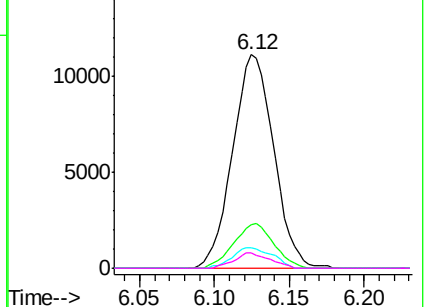

#57

4-Bromofluorobenzene

Concen: 0.810 ug/l

RT: 10.63 min Scan# 2890

Delta R.T. 0.00 min

Lab File: VU039710.D

Acq: 29 Jul 2020 18:24


Tgt Ion: 95 Resp: 6723

Ion Ratio Lower Upper

95 100

174 69.8 57.0 85.4



176 66.6 50.2 75.2

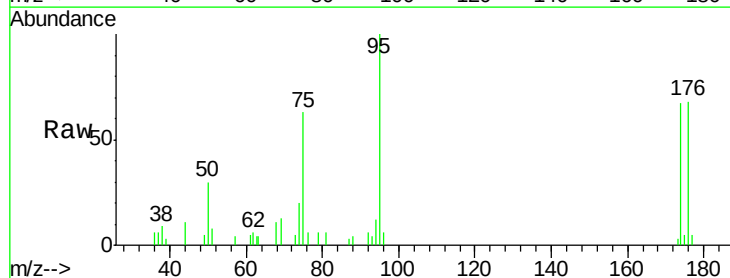


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

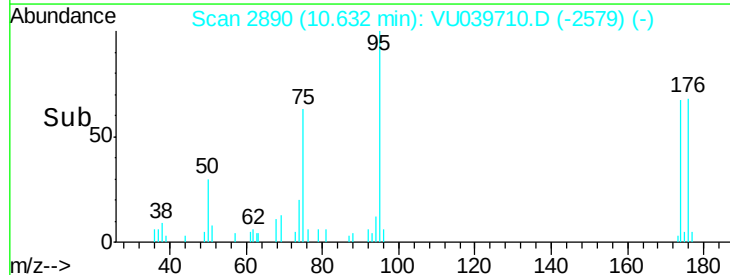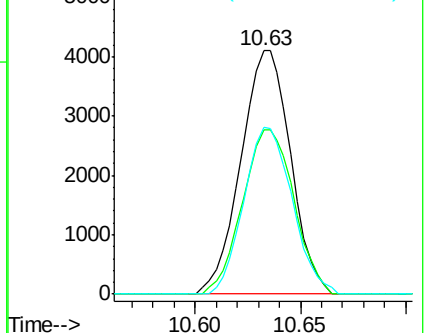

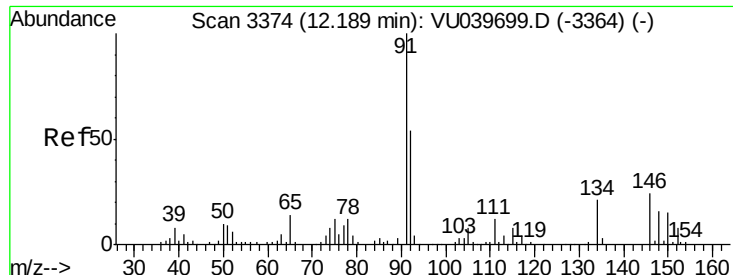

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.816 ug/l
 RT: 12.19 min Scan# 3374
 Delta R.T. 0.00 min
 Lab File: VU039710.D
 Acq: 29 Jul 2020 18:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Tot Ion	Ratio	Lower	Upper
152	100		
115	71.5	0.0	302.4
150	156.9	0.0	645.8

