


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072920\
 Data File : VU039694.D
 Acq On : 29 Jul 2020 10:10
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jul 31 07:12:27 2020

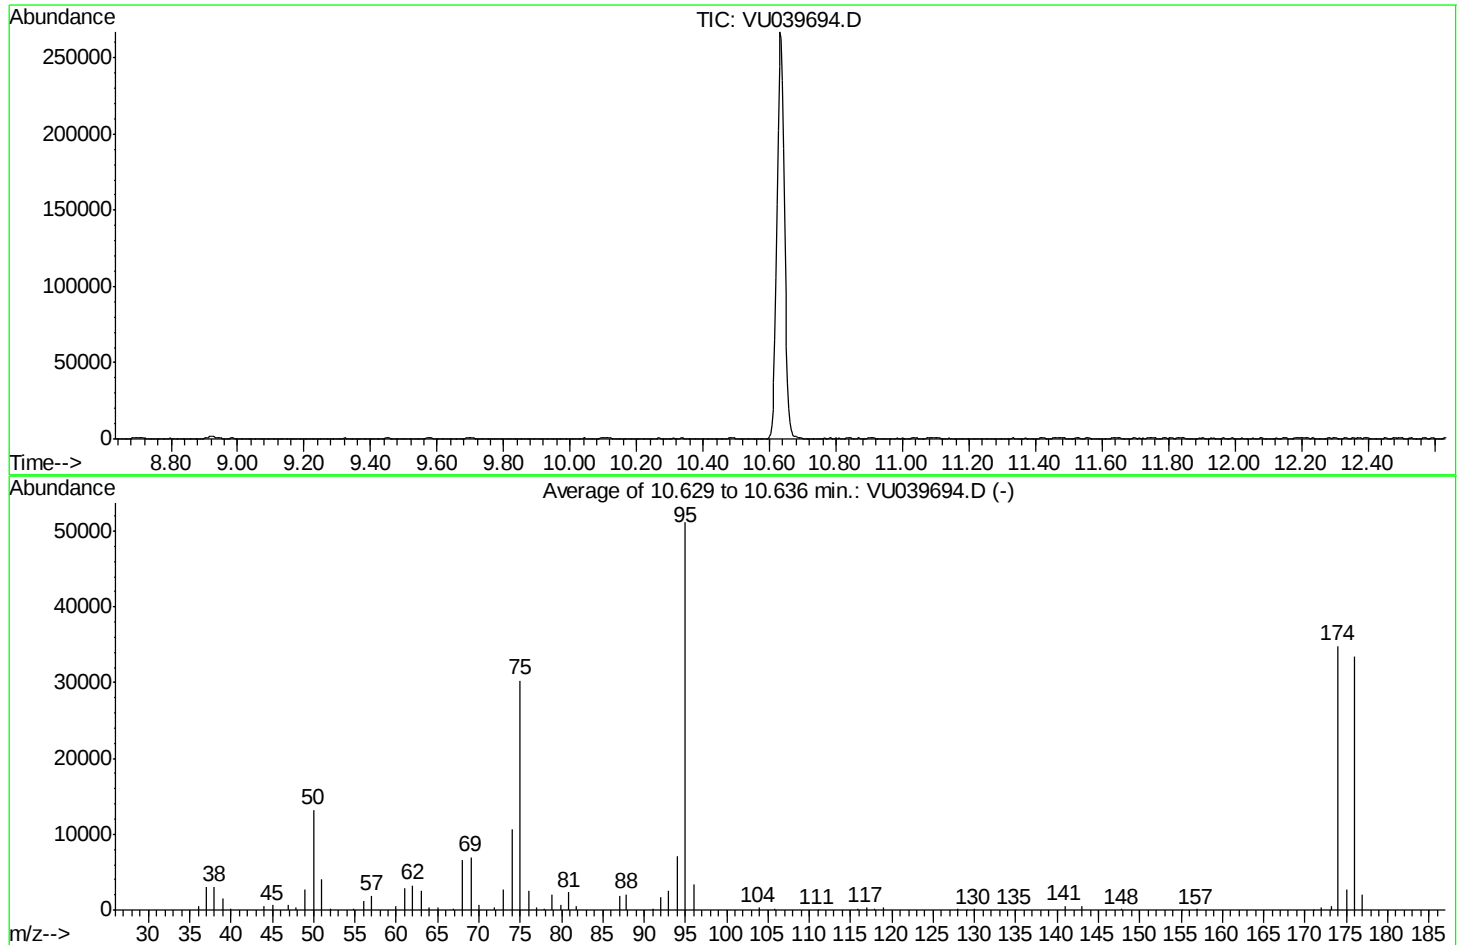

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.8	13192	PASS
75	95	30	60	59.2	30277	PASS
95	95	100	100	100.0	51165	PASS
96	95	5	9	6.6	3387	PASS
173	174	0.00	2	1.3	449	PASS
174	95	50	100	68.0	34816	PASS
175	174	5	9	7.9	2736	PASS
176	174	95	101	95.9	33373	PASS
177	176	5	9	6.1	2045	PASS