

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
 Data File : VU050026.D
 Acq On : 29 Jul 2022 10:43
 Operator : SY/MD
 Sample : VU0729WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rVB	44581	49841	12.59%	1.826%
2	1.732	115	122	130	rVB	3627	4416	1.12%	0.162%
3	1.912	170	178	189	rBV	37347	46439	11.73%	1.701%
4	2.565	369	381	398	rVB	63445	101848	25.72%	3.731%
5	3.044	521	530	541	rVB2	6107	10640	2.69%	0.390%
6	3.186	560	574	592	rVB	11686	26153	6.61%	0.958%
7	3.797	745	764	765	rBV	2283	4531	1.14%	0.166%
8	4.639	1011	1026	1056	rBV3	54583	198946	50.25%	7.288%
9	5.063	1143	1158	1176	rBV2	62535	142497	35.99%	5.220%
10	5.726	1345	1364	1389	rBV2	124811	321121	81.10%	11.763%
11	6.250	1513	1527	1554	rBV	103809	198126	50.04%	7.258%
12	6.694	1652	1665	1682	rBV	80715	155530	39.28%	5.697%
13	7.568	1925	1937	1958	rBV	37175	66404	16.77%	2.433%
14	7.899	2026	2040	2061	rBV	134040	235236	59.41%	8.617%
15	8.182	2117	2128	2147	rBV	22051	37920	9.58%	1.389%
16	8.639	2258	2270	2308	rBV4	150035	395951	100.00%	14.504%
17	9.417	2500	2512	2543	rBV	145430	250022	63.14%	9.159%
18	10.758	2915	2929	2948	rBV	67851	111790	28.23%	4.095%
19	11.812	3246	3257	3280	rVB	119335	190652	48.15%	6.984%
20	12.195	3364	3376	3392	rBV	109327	181798	45.91%	6.660%


Sum of corrected areas: 2729861

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050026.D
Acq On : 29 Jul 2022 10:43
Operator : SY/MD
Sample : VU0729WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

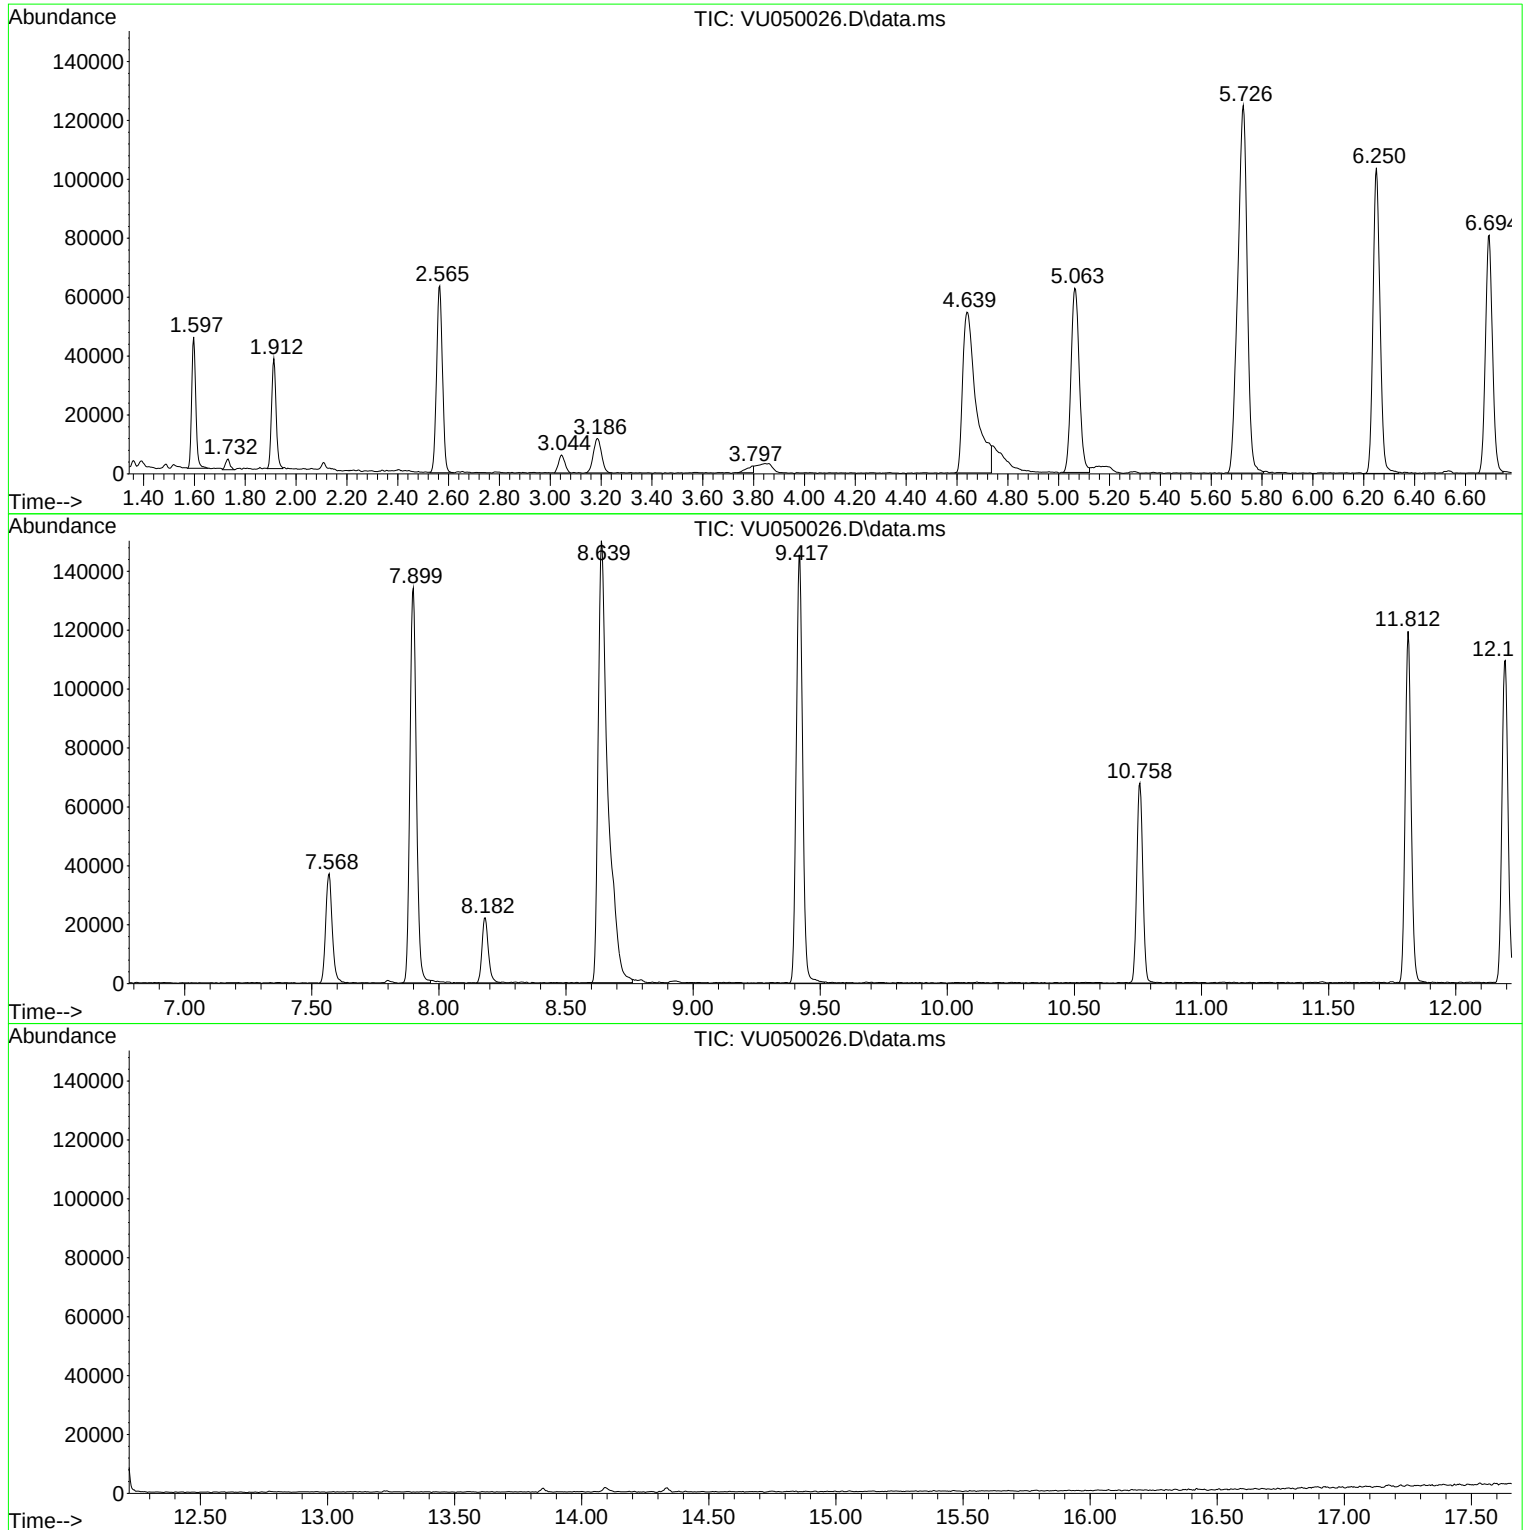

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050026.D
Acq On : 29 Jul 2022 10:43
Operator : SY/MD
Sample : VU0729WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050026.D
Acq On : 29 Jul 2022 10:43
Operator : SY/MD
Sample : VU0729WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------