

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
 Data File : VU050029.D
 Acq On : 29 Jul 2022 12:13
 Operator : SY/MD
 Sample : N3850-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU050029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	41597	46748	11.58%	1.773%
2	1.912	169	178	190	rVB	35760	45019	11.15%	1.707%
3	2.067	220	226	237	rVB	5419	5780	1.43%	0.219%
4	2.562	369	380	397	rVB	62223	98439	24.39%	3.734%
5	3.038	519	528	541	rVB3	6349	12029	2.98%	0.456%
6	3.186	561	574	588	rVB	11699	25739	6.38%	0.976%
7	3.819	753	771	773	rBV	2039	4510	1.12%	0.171%
8	4.655	1018	1031	1061	rBV2	41998	181302	44.92%	6.876%
9	5.063	1141	1158	1175	rBV2	62696	137421	34.05%	5.212%
10	5.723	1344	1363	1387	rBV2	125326	314425	77.91%	11.925%
11	6.250	1514	1527	1551	rBV	96064	179497	44.48%	6.808%
12	6.694	1651	1665	1683	rBV	80327	154315	38.24%	5.853%
13	7.565	1922	1936	1956	rBV2	36004	64703	16.03%	2.454%
14	7.899	2027	2040	2066	rBV	130214	228229	56.55%	8.656%
15	8.182	2114	2128	2142	rBV	22105	37707	9.34%	1.430%
16	8.642	2259	2271	2308	rBV4	144215	403581	100.00%	15.307%
17	9.417	2498	2512	2538	rBV	136126	225900	55.97%	8.568%
18	10.758	2918	2929	2945	rVB	69627	111587	27.65%	4.232%
19	11.812	3246	3257	3276	rBV	110720	176762	43.80%	6.704%
20	12.195	3364	3376	3395	rBV	114496	182909	45.32%	6.937%




Sum of corrected areas: 2636602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050029.D
Acq On : 29 Jul 2022 12:13
Operator : SY/MD
Sample : N3850-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

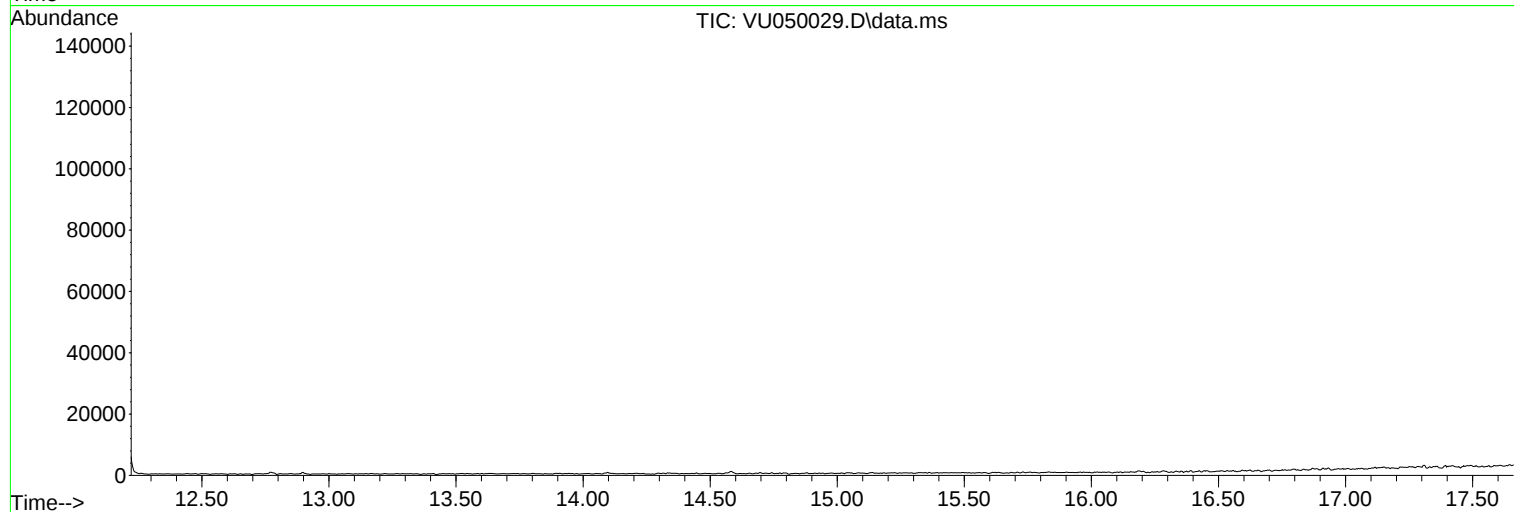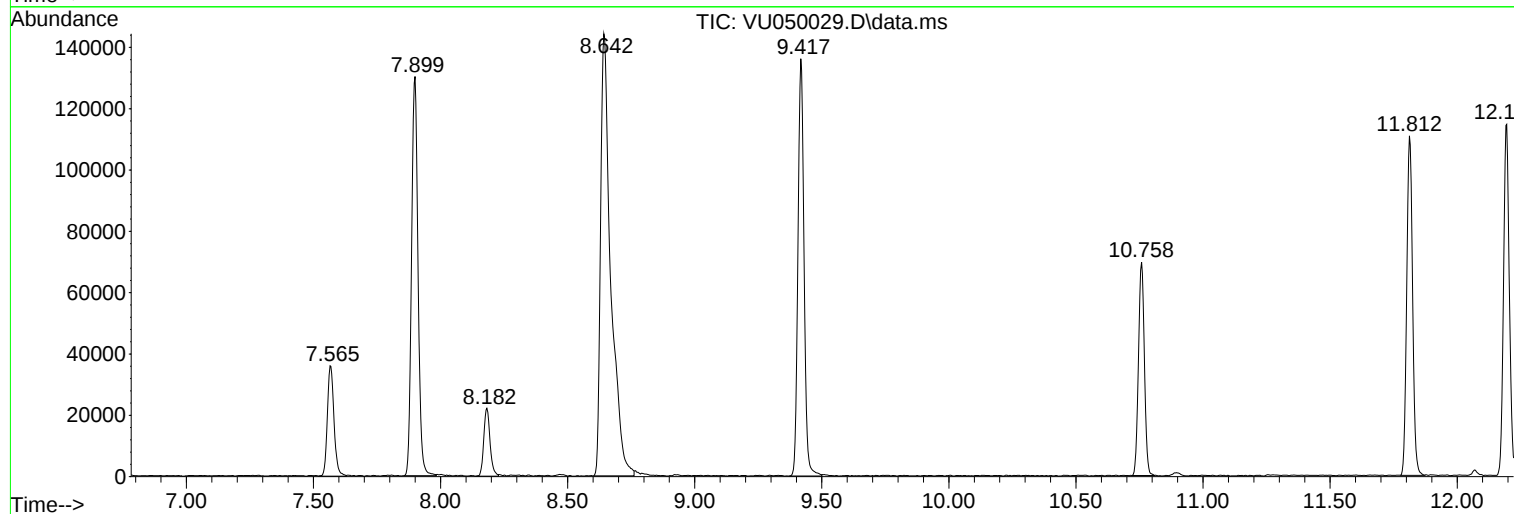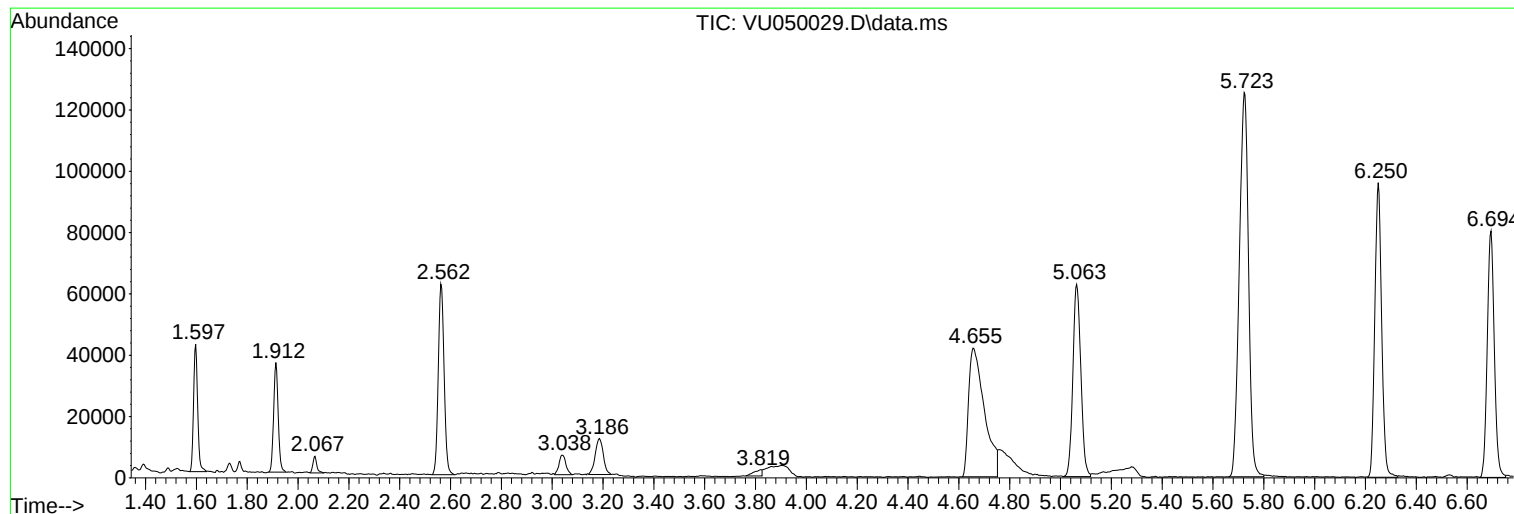

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050029.D
Acq On : 29 Jul 2022 12:13
Operator : SY/MD
Sample : N3850-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
Data File : VU050029.D
Acq On : 29 Jul 2022 12:13
Operator : SY/MD
Sample : N3850-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc