


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072922\
 Data File : VU050024.D
 Acq On : 29 Jul 2022 08:53
 Operator : SY/MD
 Sample : BFB097
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB097

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 30 01:40:38 2022

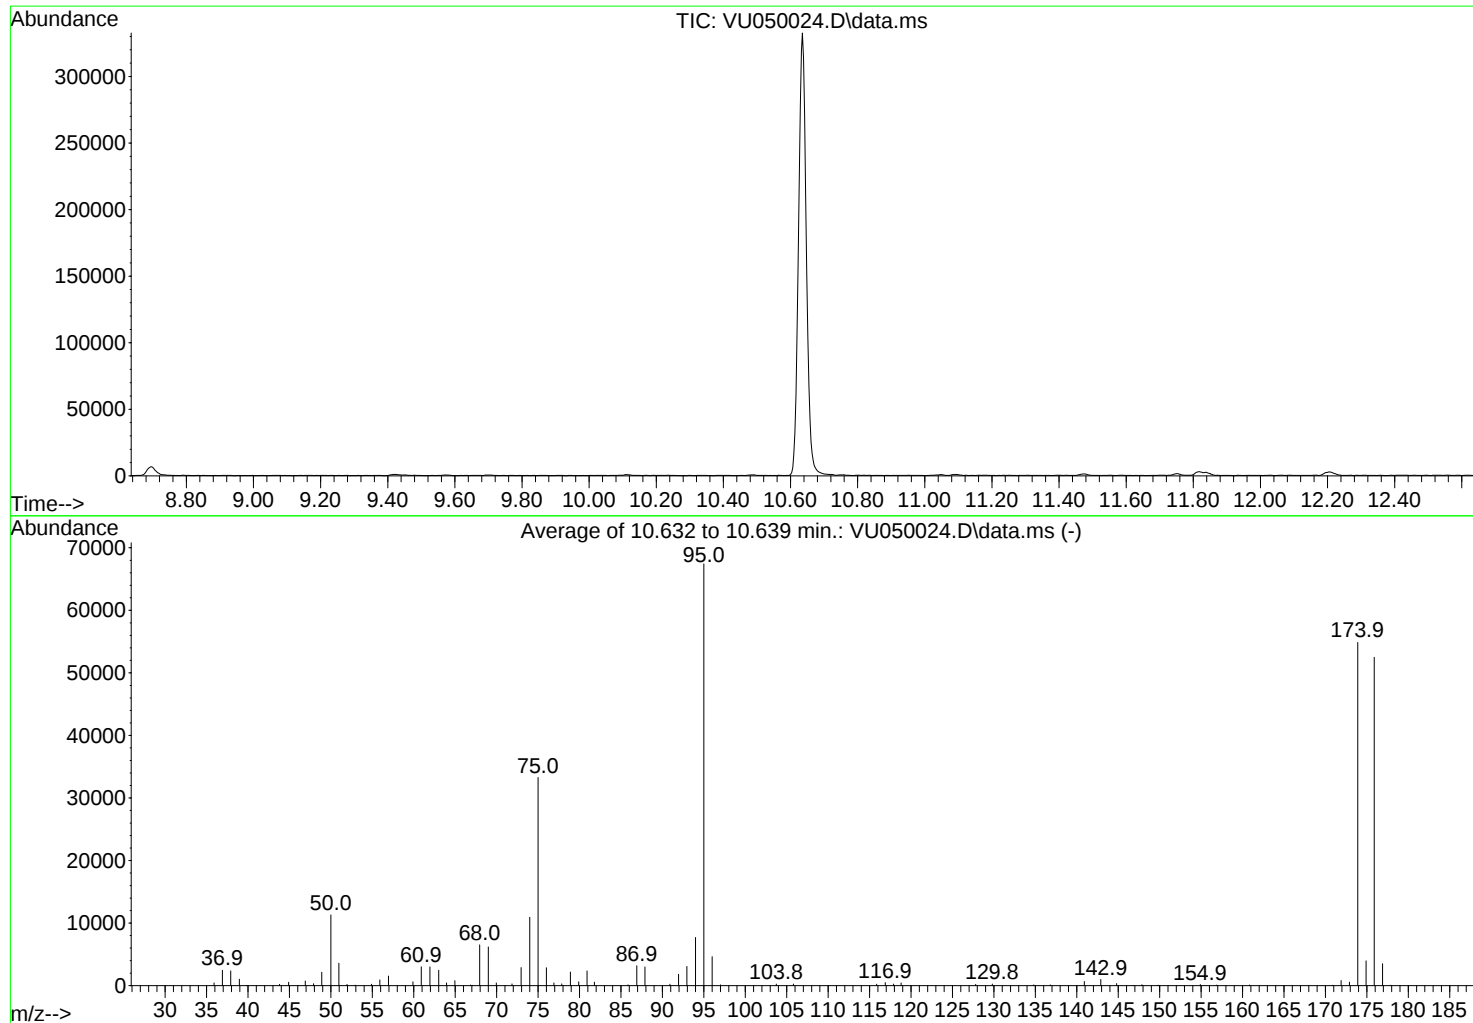

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	11303	PASS
75	95	30	80	49.4	33283	PASS
95	95	100	100	100.0	67435	PASS
96	95	5	9	6.9	4632	PASS
173	174	0.00	2	1.0	560	PASS
174	95	50	120	81.4	54875	PASS
175	174	5	9	7.2	3956	PASS
176	174	95	101	95.7	52501	PASS
177	176	5	9	6.7	3499	PASS

m/z	Abundance
39.80	116.0
43.80	267.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	464.0
36.90	2534.0
37.90	2366.0
39.00	987.0
39.80	139.0
43.90	514.0
44.90	570.0
46.90	766.0
47.90	298.0
48.90	2323.0
50.00	11473.0
50.90	3682.0
52.00	210.0
52.90	108.0
54.90	241.0
55.90	875.0
57.00	1579.0
59.90	588.0
60.90	2990.0
62.00	2988.0
63.00	2528.0
64.00	396.0
65.00	747.0
67.10	139.0
68.00	6460.0
69.00	6219.0
70.00	462.0
71.90	275.0
73.00	2897.0
74.00	10968.0
75.00	33136.0
76.00	2924.0
76.90	432.0
77.90	276.0
78.90	2206.0
79.90	573.0
80.90	2354.0
81.80	601.0
85.80	131.0
86.90	3268.0
87.90	2909.0
90.90	268.0
91.90	1883.0
93.00	3089.0
94.00	7458.0
95.00	67808.0
96.00	4679.0
97.00	112.0
103.70	245.0
105.80	253.0
115.90	209.0
116.90	495.0
117.90	266.0
118.80	460.0
127.80	197.0
129.80	264.0
134.80	129.0
136.80	109.0
140.90	647.0
142.90	943.0
144.80	329.0
147.80	166.0
154.90	151.0
156.90	117.0
160.90	140.0
171.90	851.0
172.90	534.0
173.90	53408.0
174.90	3959.0
175.90	50912.0
176.90	3457.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	446.0
36.90	2521.0
37.90	2456.0
39.00	1050.0
39.80	137.0
43.80	498.0
44.90	568.0
46.10	103.0
46.90	787.0
47.90	301.0
48.90	2196.0
50.00	11668.0
50.90	3674.0
51.90	219.0
52.90	113.0
54.90	247.0
55.90	951.0
56.90	1606.0
59.90	640.0
60.90	3149.0
61.90	3079.0
63.00	2504.0
63.90	443.0
64.90	845.0
66.80	132.0
67.90	6718.0
69.00	6333.0
69.90	465.0
71.90	292.0
73.00	2989.0
74.00	11317.0
75.00	34520.0
76.00	2933.0
76.90	474.0
77.80	313.0
78.90	2219.0
79.90	624.0
80.90	2441.0
81.80	587.0
85.80	147.0
86.90	3296.0
87.90	3067.0
90.90	239.0
91.90	1857.0
92.90	3167.0
94.00	7907.0
95.00	69616.0
96.00	4777.0
97.00	114.0
103.80	277.0
105.80	254.0
115.90	233.0
116.90	487.0
117.90	274.0
118.80	467.0
127.80	195.0
129.80	267.0
134.80	125.0
136.80	132.0
140.90	710.0
142.90	1038.0
144.80	346.0
146.80	103.0
147.80	148.0
149.80	109.0
154.90	199.0
156.90	117.0
160.80	137.0
170.90	111.0
171.90	813.0
172.90	571.0
173.90	56624.0
174.90	4127.0
175.90	54240.0
176.90	3641.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097

m/z	Abundance
35.90	409.0
36.90	2356.0
37.90	2246.0
38.90	1032.0
39.80	149.0
43.80	447.0
44.90	503.0
46.90	703.0
47.90	288.0
48.90	1967.0
50.00	10768.0
51.00	3393.0
52.00	207.0
54.90	227.0
55.90	919.0
56.90	1396.0
59.90	628.0
60.90	2901.0
61.90	2930.0
63.00	2317.0
63.90	440.0
64.90	811.0
66.90	147.0
67.90	6388.0
69.00	6020.0
69.90	406.0
71.80	313.0
72.90	2778.0
74.00	10469.0
75.00	32192.0
76.00	2728.0
76.90	437.0
77.80	293.0
78.90	2084.0
79.90	631.0
80.90	2270.0
81.80	546.0
85.90	139.0
86.90	2958.0
87.90	2996.0
90.90	214.0
92.00	1739.0
92.90	2977.0
94.00	7744.0
95.00	64880.0
96.00	4440.0
97.00	130.0
103.80	285.0
105.80	263.0
115.80	245.0
116.90	469.0
117.90	273.0
118.80	390.0
127.80	205.0
129.80	237.0
134.80	104.0
136.80	135.0
140.90	670.0
142.90	996.0
144.80	296.0
147.90	129.0
149.80	104.0
154.90	212.0
156.90	108.0
170.90	118.0
171.90	764.0
172.90	576.0
173.90	54592.0
174.90	3782.0
175.90	52352.0
176.90	3398.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB097