




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060250.D
Acq On : 29 Jul 2024 14:55
Operator : MD/SY
Sample : P3359-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC1

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:22:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

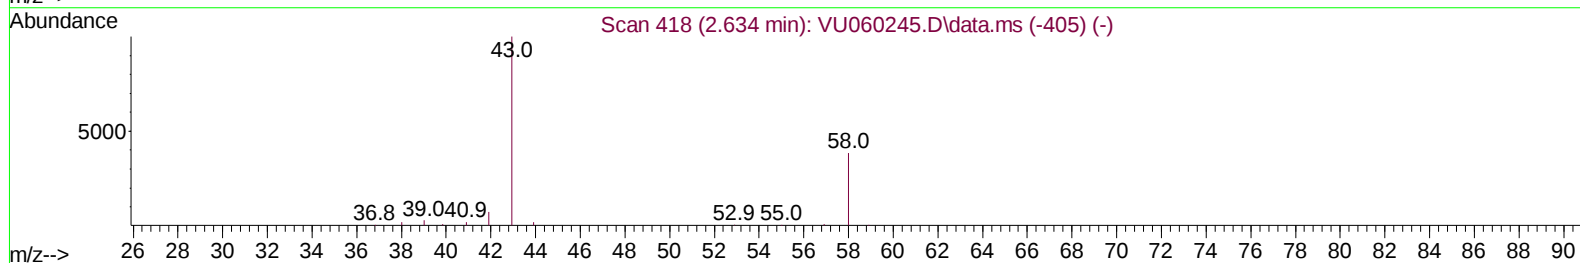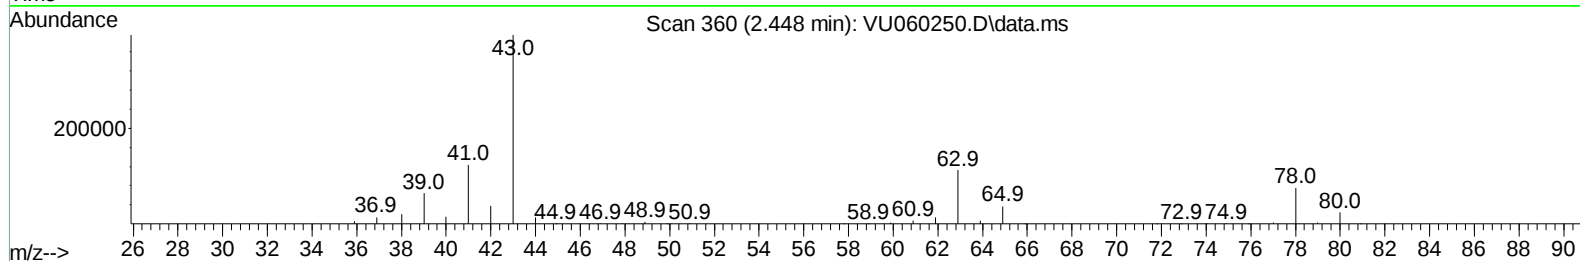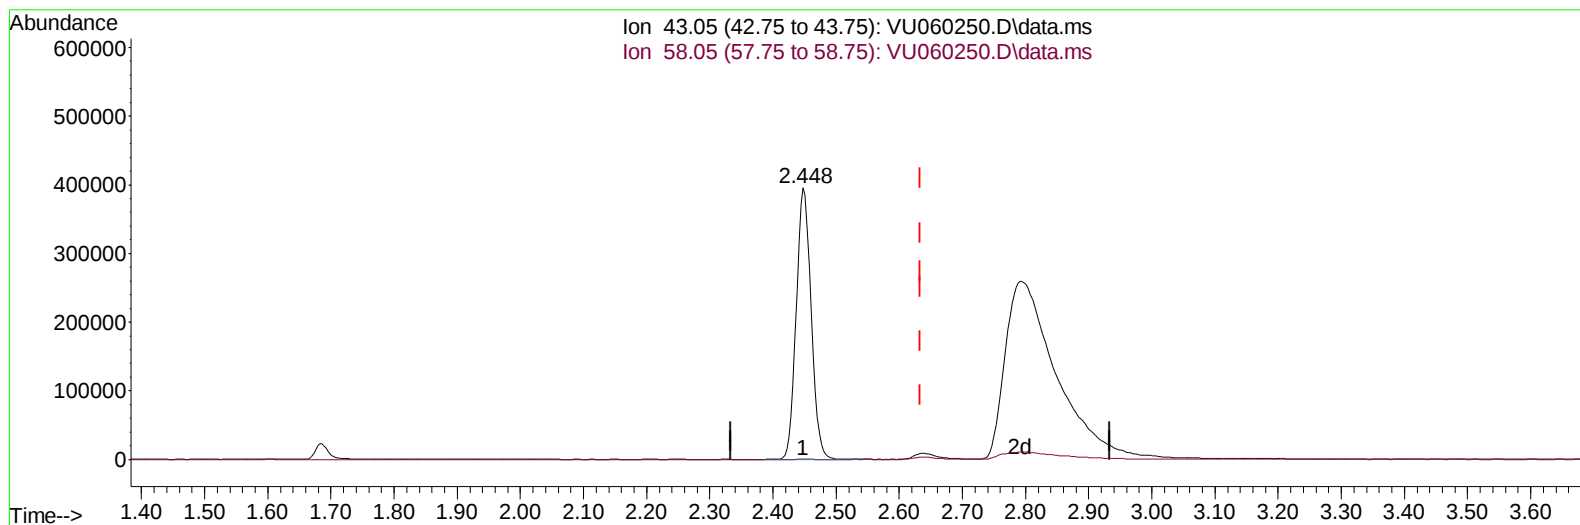

TIC: VU060250.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 458.95 ug/L

response 649326

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060250.D
Acq On : 29 Jul 2024 14:55
Operator : MD/SY
Sample : P3359-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 30 04:22:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

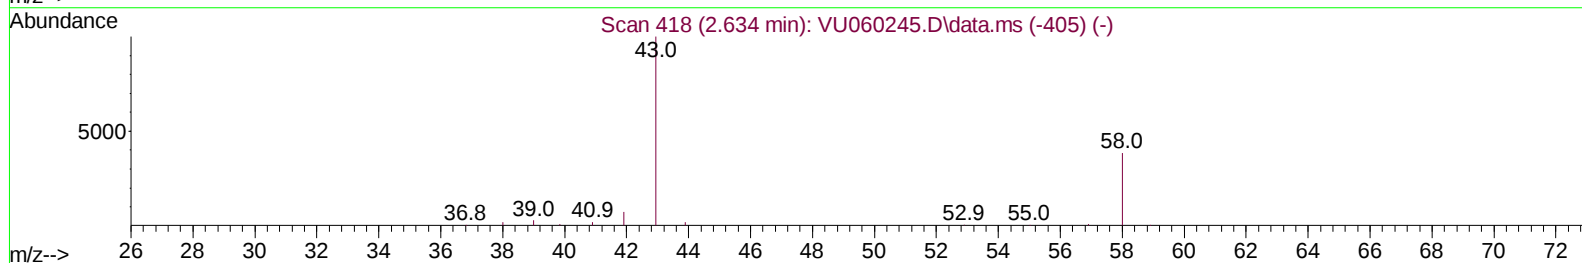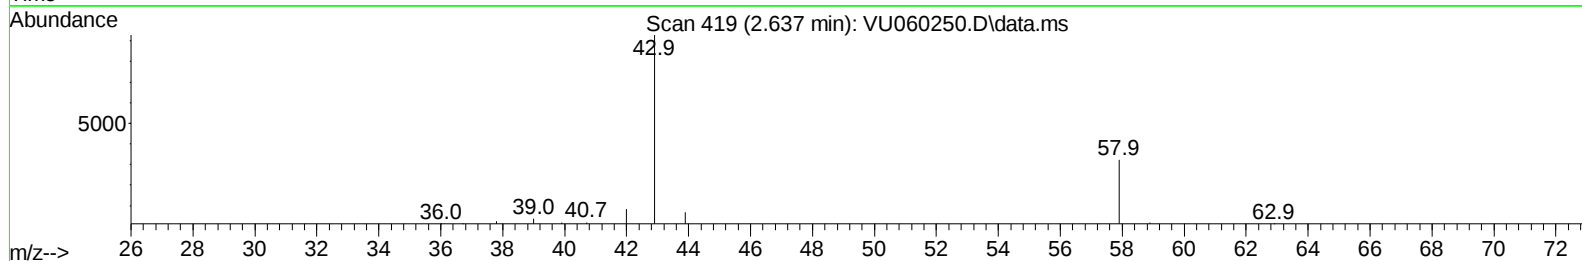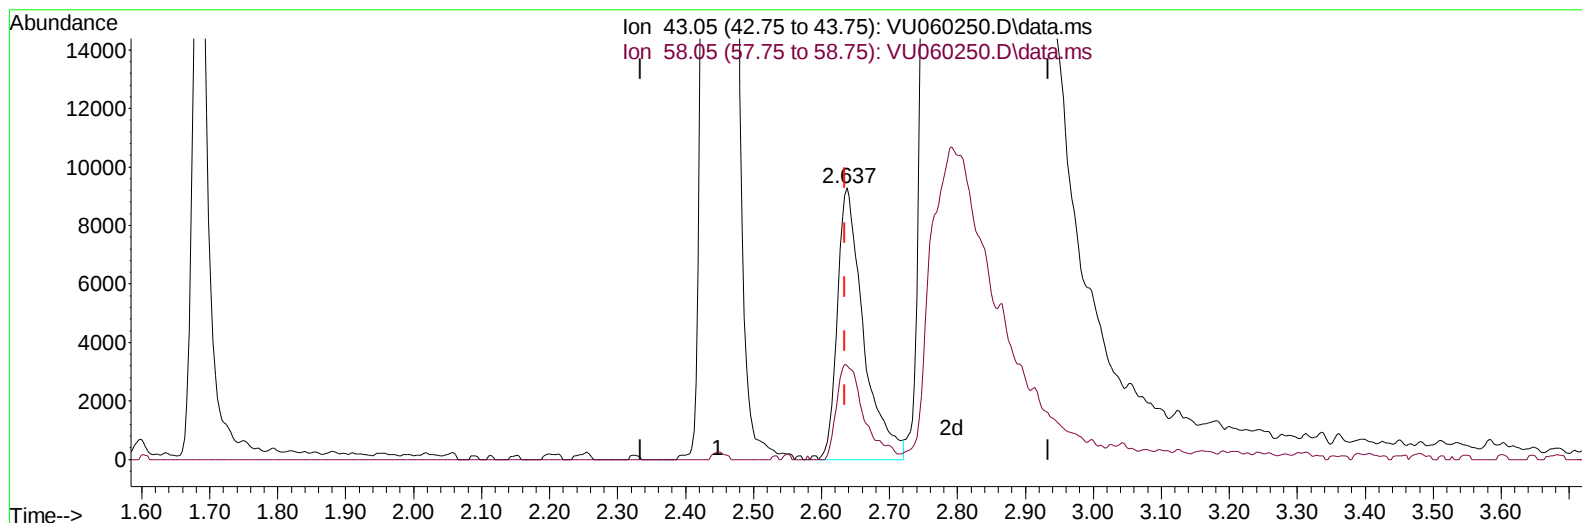

TIC: VU060250.D\data.ms

(13) Acetone (T)

2.637min (+ 0.003) 17.57 ug/L m

response 24859

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	36.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
 Data File : VU060250.D
 Acq On : 29 Jul 2024 14:55
 Operator : MD/SY
 Sample : P3359-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GC1

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:22:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 30 04:21:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		131485	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		140736	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		58378	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		36714	4.013	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	80.200%		
7) Chloroethane-d5	1.907	69		38144	4.488	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	89.800%		
11) 1,1-Dichloroethene-d2	2.560	65		14971	4.191	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	83.800%		
20) 2-Butanone-d5	4.621	46		150459	70.347	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	140.700%#		
24) Chloroform-d	5.055	84		92870	4.830	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	96.600%		
26) 1,2-Dichloroethane-d4	5.695	65		47884	5.349	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	107.000%		
32) Benzene-d6	5.721	84		163445	4.335	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	86.600%		
36) 1,2-Dichloropropane-d6	6.685	67		61224	5.095	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	102.000%		
41) Toluene-d8	7.894	98		120846	3.547	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	71.000%		
43) trans-1,3-Dichloroprop...	8.177	79		17923	4.382	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	87.600%		
46) 2-Hexanone-d5	8.627	63		99509	54.827	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	109.660%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		59194	5.535	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	110.800%		
66) 1,2-Dichlorobenzene-d4	12.190	152		56108	5.325	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	106.400%		
Target Compounds							
13) Acetone	2.637	43		24859m	17.570	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060250.D
Acq On : 29 Jul 2024 14:55
Operator : MD/SY
Sample : P3359-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 30 04:22:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

