




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060252.D
Acq On : 29 Jul 2024 15:42
Operator : MD/SY
Sample : P3359-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF6

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:23:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

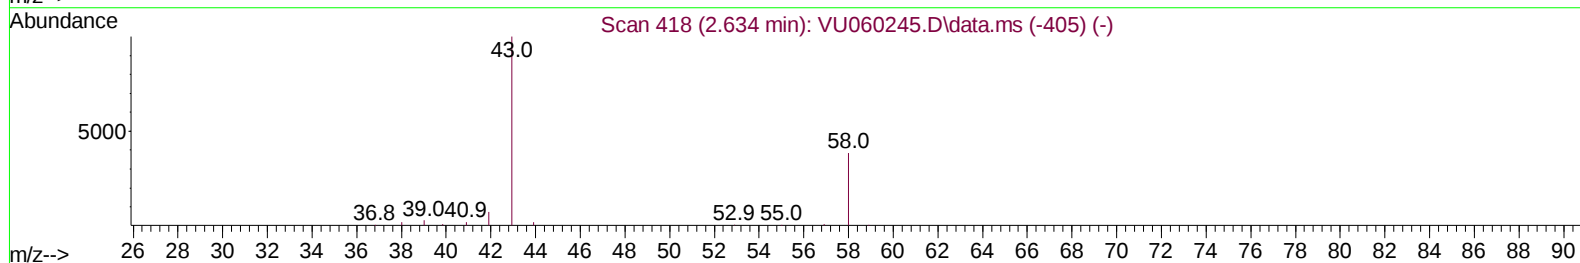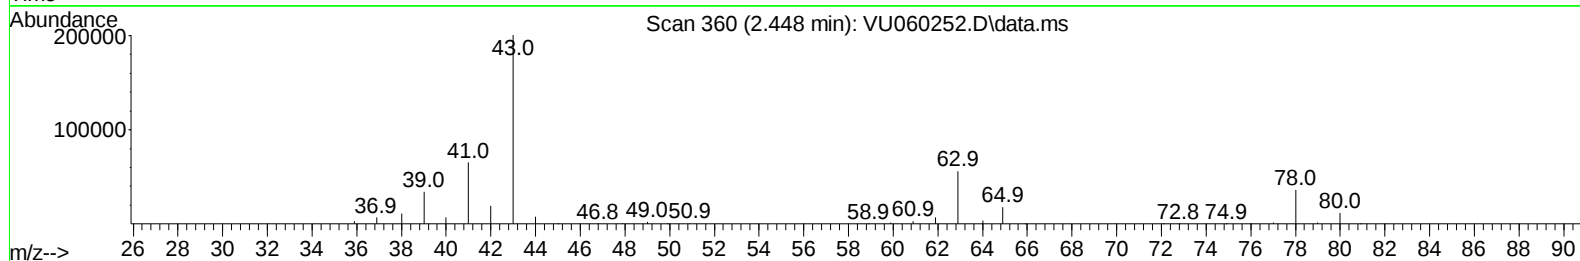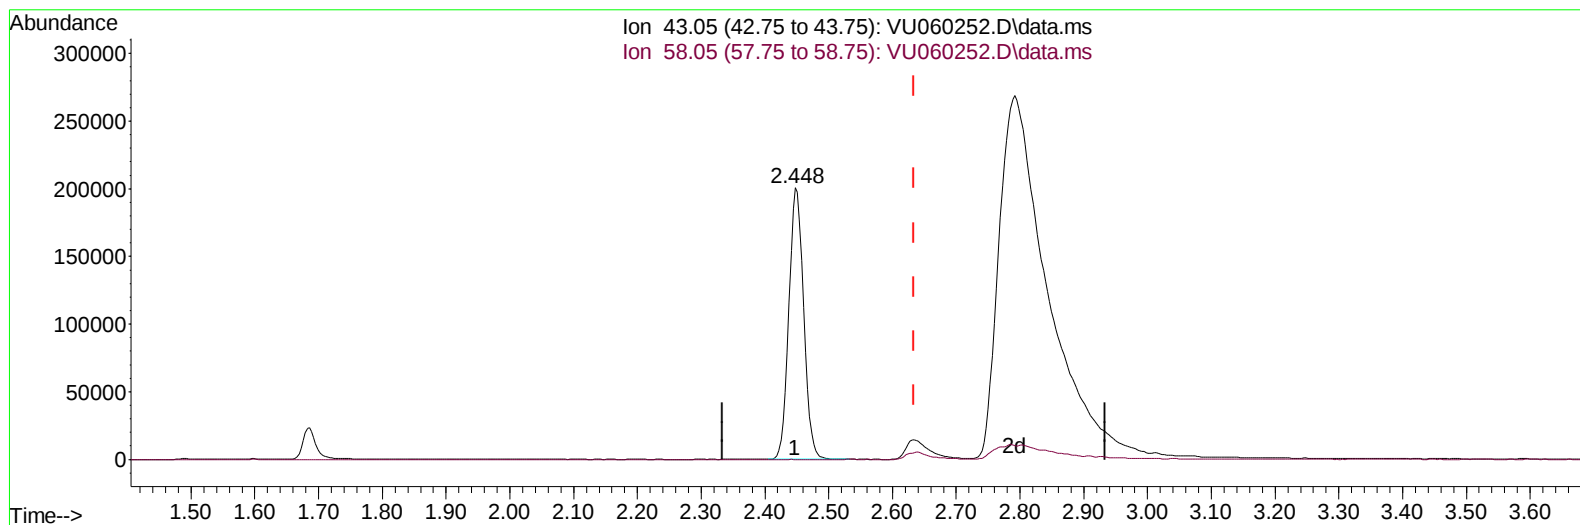

TIC: VU060252.D\data.ms

(13) Acetone (T)

2.448min (-0.187) 221.84 ug/L

response 323793

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	4.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060252.D
Acq On : 29 Jul 2024 15:42
Operator : MD/SY
Sample : P3359-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF6

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:23:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

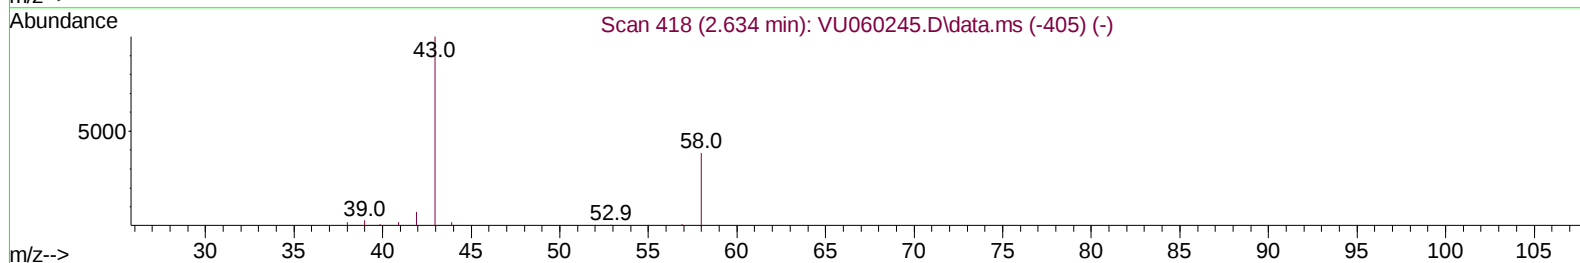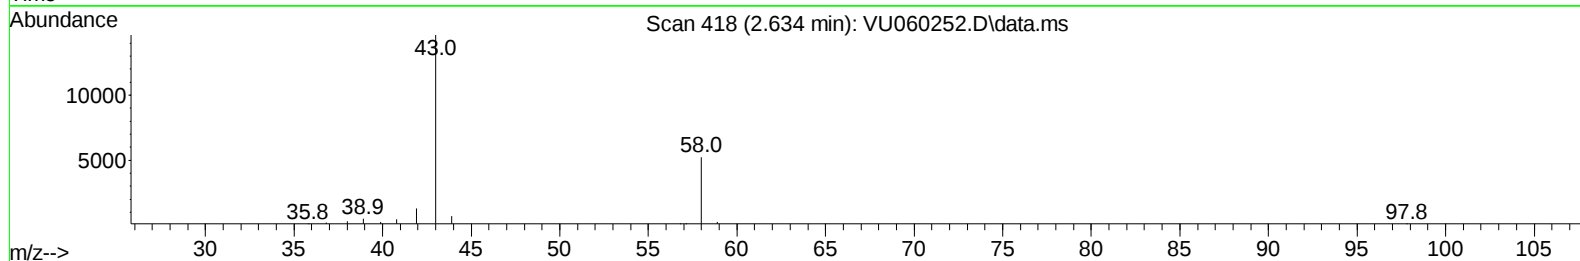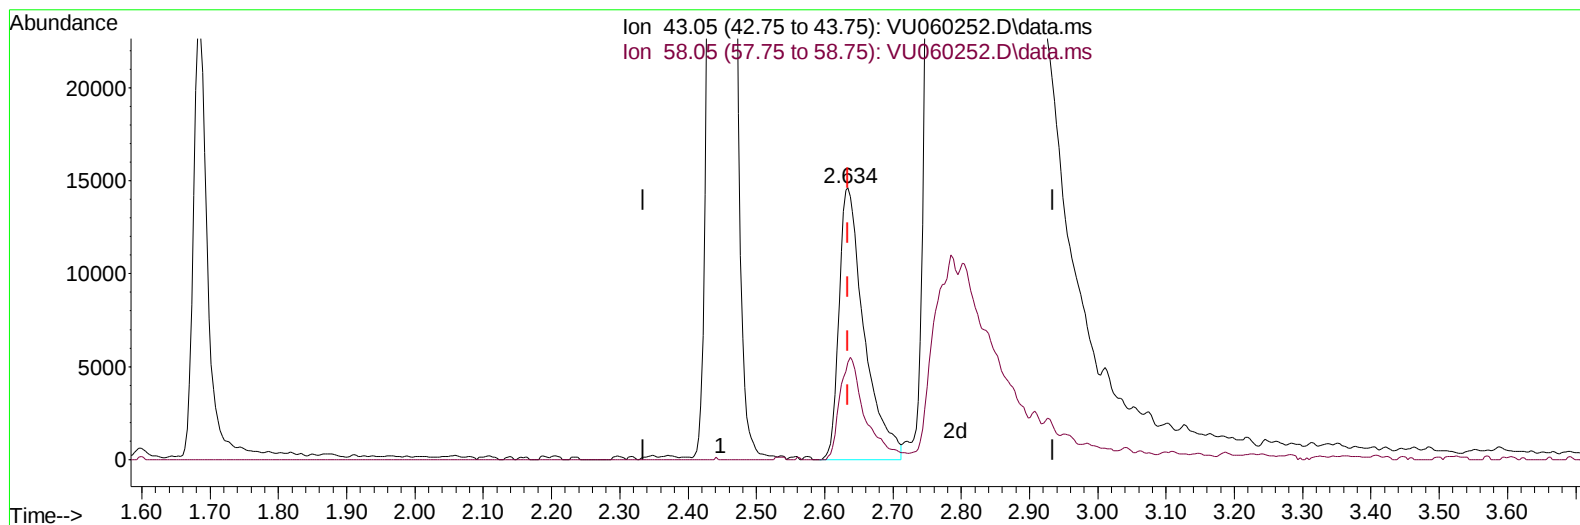

TIC: VU060252.D\data.ms

(13) Acetone (T)

2.634min (-0.000) 25.67 ug/L m

response 37468

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	38.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
 Data File : VU060252.D
 Acq On : 29 Jul 2024 15:42
 Operator : MD/SY
 Sample : P3359-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF6

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:23:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 30 04:21:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		135645	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		144150	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		61320	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		35305	3.741	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	74.800%		
7) Chloroethane-d5	1.911	69		37101	4.232	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	84.600%		
11) 1,1-Dichloroethene-d2	2.560	65		13827	3.752	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	75.000%		
20) 2-Butanone-d5	4.621	46		141935	64.327	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	128.660%		
24) Chloroform-d	5.055	84		88797	4.477	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.600%		
26) 1,2-Dichloroethane-d4	5.695	65		44852	4.856	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	97.200%		
32) Benzene-d6	5.721	84		154213	3.993	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	79.800%		
36) 1,2-Dichloropropane-d6	6.685	67		59458	4.831	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	96.600%		
41) Toluene-d8	7.894	98		113478	3.252	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	65.000%#		
43) trans-1,3-Dichloroprop...	8.177	79		17706	4.227	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	84.600%		
46) 2-Hexanone-d5	8.627	63		97293	52.337	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	104.680%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		56095	5.121	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	102.400%		
66) 1,2-Dichlorobenzene-d4	12.187	152		54054	4.884	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	97.600%		
Target Compounds							
13) Acetone	2.634	43		37468m	25.670	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060252.D
Acq On : 29 Jul 2024 15:42
Operator : MD/SY
Sample : P3359-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF6

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 30 04:23:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 30 04:21:24 2024
Response via : Initial Calibration

