
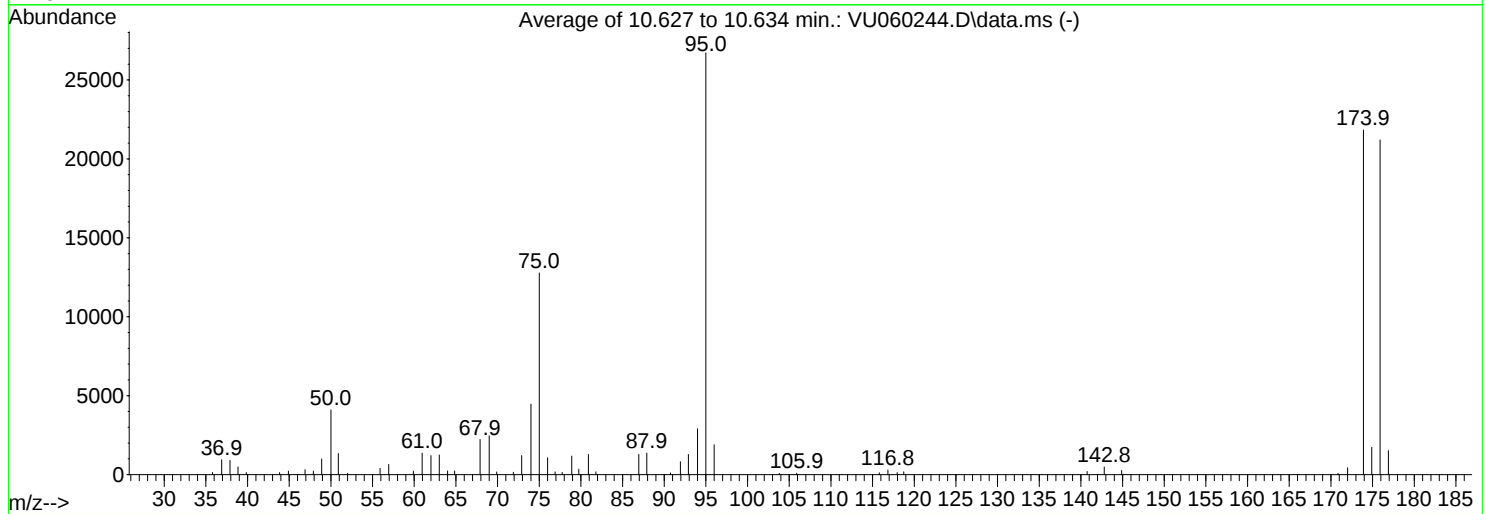


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072924\
Data File : VU060244.D
Acq On : 29 Jul 2024 09:33
Operator : MD/SY
Sample : BFB180
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB180

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jul 30 04:21:24 2024

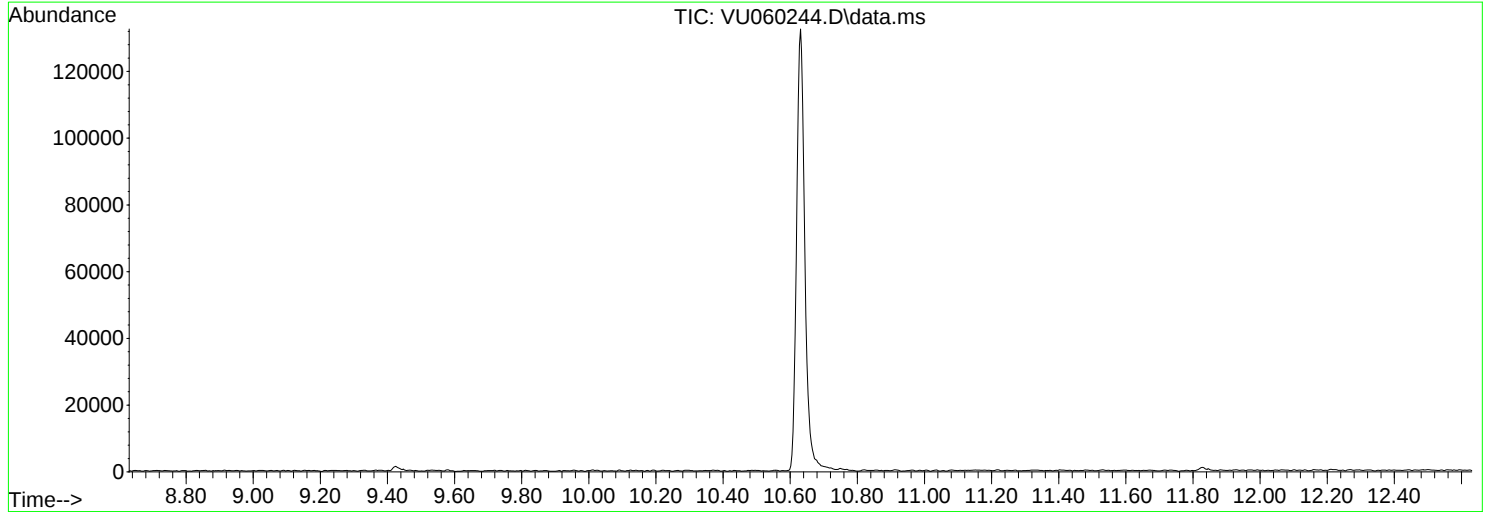

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	4103	PASS
75	95	30	80	47.8	12784	PASS
95	95	100	100	100.0	26717	PASS
96	95	5	9	7.1	1895	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.7	21832	PASS
175	174	5	9	7.9	1735	PASS
176	174	95	101	97.1	21200	PASS
177	176	5	9	7.2	1521	PASS

m/z	Abundance
43.90	334.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
35.90	127.0
36.90	895.0
37.90	959.0
38.80	482.0
39.80	129.0
43.80	450.0
44.90	240.0
46.90	325.0
47.90	229.0
48.90	1022.0
50.00	4068.0
50.90	1326.0
52.00	149.0
55.90	438.0
57.00	640.0
59.90	264.0
61.00	1277.0
62.00	1246.0
63.00	1308.0
64.00	213.0
64.90	222.0
67.90	2133.0
69.00	2507.0
69.90	123.0
71.90	259.0
72.90	1120.0
74.00	4525.0
75.00	12513.0
76.00	1189.0
76.90	165.0
77.70	119.0
78.90	1168.0
79.70	305.0
80.90	1300.0
81.80	163.0
86.90	1192.0
87.90	1407.0
90.80	108.0
92.00	867.0
92.90	1206.0
94.00	2896.0
95.00	26792.0
96.00	1840.0
115.90	111.0
116.80	242.0
118.00	107.0
118.80	169.0
140.80	179.0
142.80	474.0
144.90	228.0
172.00	419.0
173.90	21408.0
174.90	1714.0
175.90	21248.0
176.90	1558.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
35.90	143.0
36.90	930.0
37.90	940.0
38.90	517.0
39.90	127.0
43.80	457.0
44.90	239.0
46.90	310.0
47.90	244.0
48.90	1026.0
50.00	4242.0
50.90	1386.0
52.00	109.0
55.90	417.0
57.00	680.0
59.90	216.0
61.00	1378.0
62.00	1230.0
63.00	1292.0
64.00	246.0
64.80	230.0
67.90	2299.0
69.00	2529.0
69.90	167.0
71.90	193.0
72.90	1253.0
74.00	4562.0
75.00	13212.0
76.00	1101.0
76.90	201.0
77.80	146.0
78.90	1201.0
79.80	358.0
80.90	1296.0
81.80	188.0
87.00	1289.0
87.90	1397.0
90.70	124.0
91.90	856.0
92.90	1364.0
94.00	2948.0
95.00	27512.0
96.00	1956.0
103.80	107.0
105.90	121.0
115.80	125.0
116.90	315.0
117.90	135.0
118.70	179.0
140.70	199.0
142.80	515.0
144.90	280.0
170.90	109.0
172.00	477.0
173.90	22560.0
174.90	1779.0
175.90	21688.0
176.90	1580.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180

m/z	Abundance
35.80	154.0
36.90	1001.0
37.90	802.0
38.90	468.0
39.90	136.0
43.90	488.0
44.90	195.0
46.90	298.0
47.90	207.0
48.90	941.0
50.00	3999.0
50.90	1304.0
55.90	358.0
56.90	614.0
59.90	204.0
60.90	1416.0
62.00	1136.0
63.00	1136.0
64.00	253.0
64.80	263.0
67.90	2252.0
69.00	2352.0
69.90	224.0
72.90	1241.0
74.00	4314.0
75.00	12627.0
76.00	907.0
76.90	196.0
77.80	171.0
78.90	1149.0
79.80	377.0
80.90	1224.0
81.80	202.0
87.00	1371.0
87.90	1312.0
90.70	115.0
91.90	738.0
92.90	1273.0
94.00	2870.0
95.00	25848.0
96.00	1888.0
103.80	145.0
105.90	147.0
115.70	133.0
116.90	332.0
117.90	144.0
118.70	194.0
140.70	221.0
142.80	483.0
144.90	291.0
170.80	139.0
172.00	427.0
173.90	21528.0
174.90	1712.0
175.90	20664.0
176.90	1426.0

Instrument :
MSVOA_U
ClientSampleId :
BFB180