


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU073018\
Data File : VU025712.D
Acq On : 30 Jul 2018 09:39
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Title : SW846 8260
Last Update : Fri Jul 27 13:11:52 2018

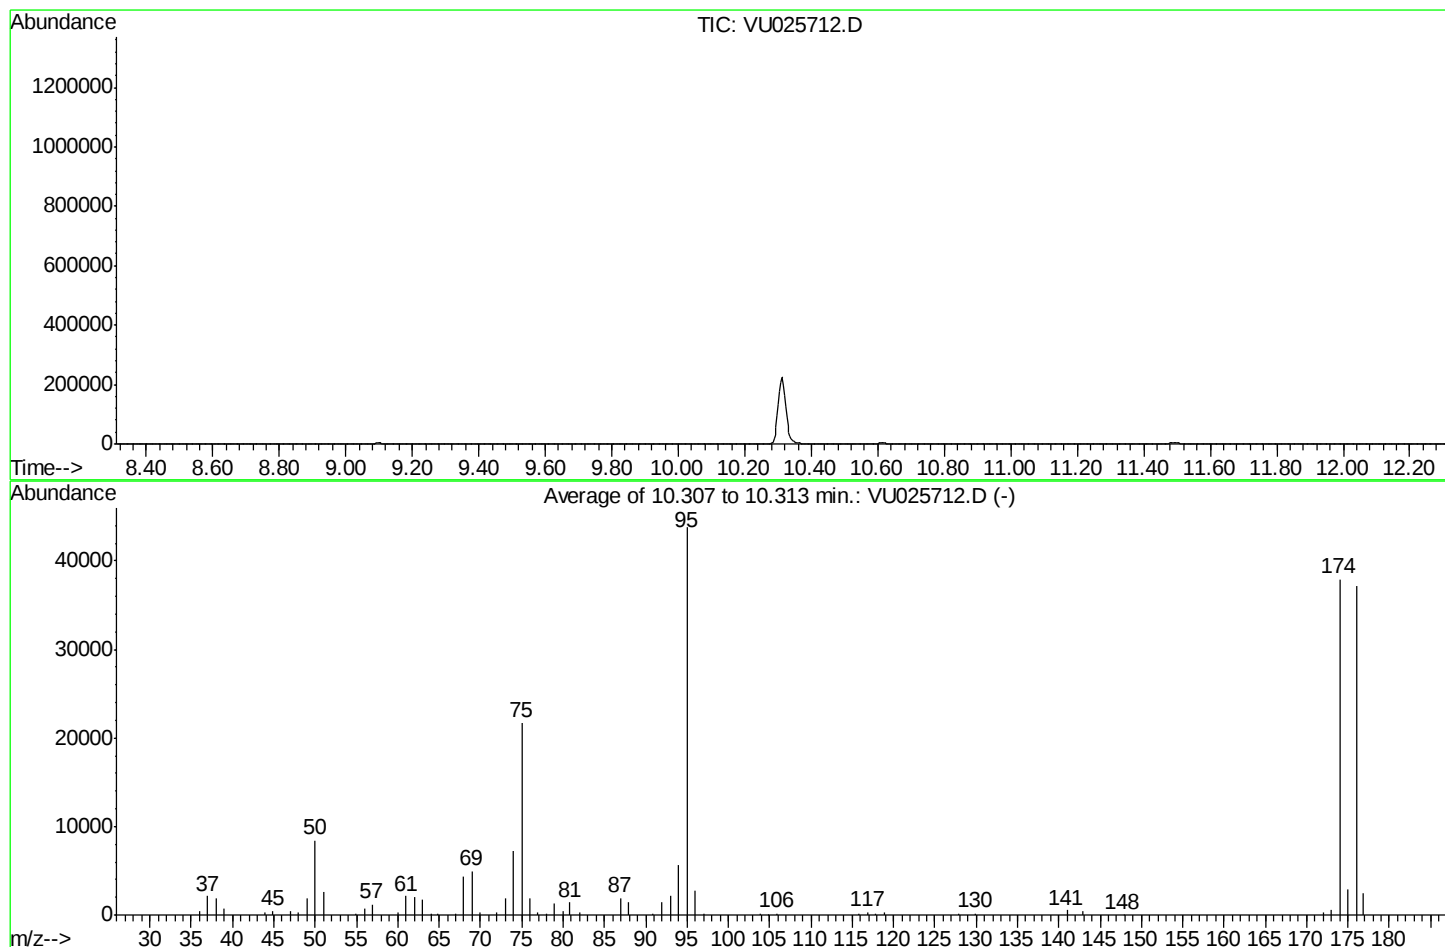

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8439	PASS
75	95	30	60	49.7	21765	PASS
95	95	100	100	100.0	43800	PASS
96	95	5	9	6.4	2815	PASS
173	174	0.00	2	1.4	522	PASS
174	95	50	100	86.7	37965	PASS
175	174	5	9	7.6	2871	PASS
176	174	95	101	97.9	37181	PASS
177	176	5	9	6.5	2427	PASS