


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU073019\
Data File : VU033480.D
Acq On : 30 Jul 2019 08:47
Operator : JC/SP
Sample : BFB41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM072919W.M
Title : VOC Analysis
Last Update : Wed Jul 31 08:44:45 2019

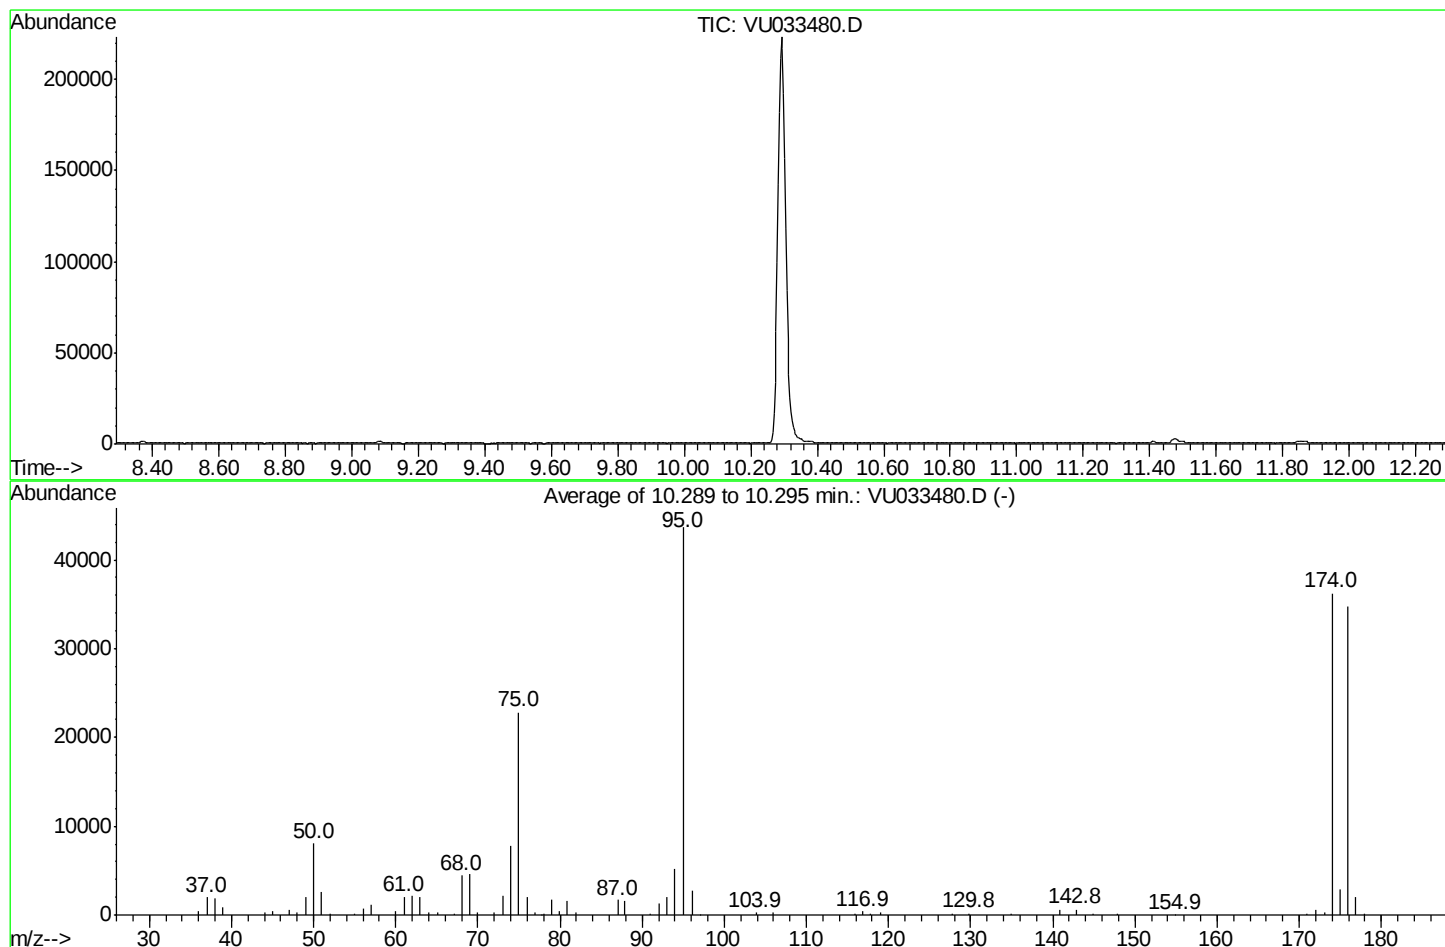

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	8014	PASS
75	95	30	80	52.2	22781	PASS
95	95	100	100	100.0	43661	PASS
96	95	5	9	6.4	2801	PASS
173	174	0.00	2	0.7	237	PASS
174	95	50	120	83.0	36232	PASS
175	174	5	9	8.0	2884	PASS
176	174	95	101	96.1	34802	PASS
177	176	5	9	6.0	2078	PASS

Scan 2850 (10.254 min): VU033480.D
BFB41

m/z	Abundance
40.00	150.0
44.00	328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	358.0
37.00	2077.0
38.00	1674.0
39.00	942.0
39.90	144.0
44.00	628.0
44.90	420.0
47.00	540.0
47.90	241.0
49.00	1932.0
50.00	7804.0
51.00	2560.0
51.90	112.0
55.00	162.0
56.00	702.0
57.00	1171.0
59.90	412.0
61.00	1978.0
62.10	2236.0
63.00	2011.0
64.00	292.0
65.00	344.0
67.10	137.0
68.00	4437.0
69.00	4595.0
70.00	345.0
72.00	355.0
73.00	2184.0
74.00	7307.0
75.00	22288.0
76.00	1996.0
76.90	224.0
77.70	198.0
78.90	1725.0
79.90	399.0
80.90	1596.0
81.90	329.0
87.00	1776.0
87.90	1644.0
90.90	220.0
92.00	1376.0
93.00	1969.0
94.00	5001.0
95.00	42760.0
96.10	2833.0
97.00	100.0
103.90	196.0
105.90	206.0
115.90	187.0
116.90	412.0
117.80	168.0
118.90	254.0
127.80	131.0
129.80	134.0
134.80	111.0
140.90	546.0
142.80	565.0
144.90	137.0
147.80	175.0
154.90	107.0
172.00	521.0
174.00	34776.0
175.00	2764.0
175.90	33264.0
176.90	2016.0
177.90	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	370.0
37.00	2034.0
38.00	1888.0
39.00	977.0
39.90	139.0
44.00	662.0
45.00	422.0
47.00	618.0
48.00	284.0
49.00	2076.0
50.00	8183.0
51.00	2663.0
51.90	134.0
54.90	132.0
56.00	756.0
57.00	1267.0
59.90	400.0
61.00	2129.0
62.10	2205.0
63.00	2041.0
64.00	309.0
65.00	334.0
67.20	165.0
68.00	4562.0
69.00	4749.0
70.00	351.0
72.00	367.0
73.00	2262.0
74.00	8018.0
75.00	23432.0
76.00	2026.0
77.00	295.0
78.90	1806.0
79.90	446.0
80.90	1615.0
81.90	357.0
87.00	1729.0
87.90	1644.0
90.90	235.0
92.00	1350.0
93.00	2095.0
94.00	5294.0
95.00	44896.0
96.10	2843.0
103.90	252.0
105.90	225.0
116.00	210.0
116.90	402.0
117.90	172.0
119.00	233.0
127.80	170.0
129.80	159.0
134.90	120.0
140.90	576.0
142.80	554.0
144.90	177.0
147.80	168.0
171.00	102.0
171.90	550.0
174.00	37504.0
175.00	2945.0
175.90	35832.0
176.90	2141.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	380.0
37.00	1800.0
38.00	1886.0
39.00	832.0
39.90	119.0
44.00	702.0
45.00	394.0
47.00	618.0
48.00	293.0
49.00	1878.0
50.00	8055.0
51.00	2522.0
52.00	129.0
54.90	100.0
56.00	776.0
57.00	1196.0
60.00	317.0
61.00	2070.0
62.00	2110.0
63.00	1949.0
64.10	274.0
65.10	337.0
67.20	152.0
68.00	4386.0
69.00	4434.0
70.00	351.0
72.00	303.0
73.00	2058.0
74.00	7913.0
75.00	22624.0
76.00	1849.0
77.00	329.0
78.10	238.0
78.90	1722.0
79.90	442.0
80.90	1484.0
81.90	352.0
87.00	1625.0
87.90	1627.0
90.90	205.0
92.00	1268.0
93.00	1915.0
94.00	5149.0
95.00	43328.0
96.10	2729.0
103.90	248.0
105.90	237.0
116.00	197.0
116.90	380.0
117.90	159.0
119.00	228.0
127.80	160.0
129.80	170.0
134.90	126.0
140.90	549.0
142.90	617.0
144.80	189.0
147.90	139.0
170.90	132.0
171.90	566.0
173.10	711.0
174.00	36416.0
175.00	2943.0
175.90	35312.0
176.90	2078.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41