

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073020\
 Data File : VU039718.D
 Acq On : 30 Jul 2020 12:19
 Operator : SY/MD
 Sample : VU0730WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0730WBL01

Quant Time: Jul 31 06:31:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 30 13:49:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	6.13	96	26489	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.63	95	7587	0.73	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.00%	
68) 1,2-Dichlorobenzene-d4	12.19	152	7224	0.71	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU073020\
Data File : VU039718.D
Acq On : 30 Jul 2020 12:19
Operator : SY/MD
Sample : VU0730WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0730WBL01

Quant Time: Jul 31 06:31:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072920DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 30 13:49:19 2020
Response via : Initial Calibration

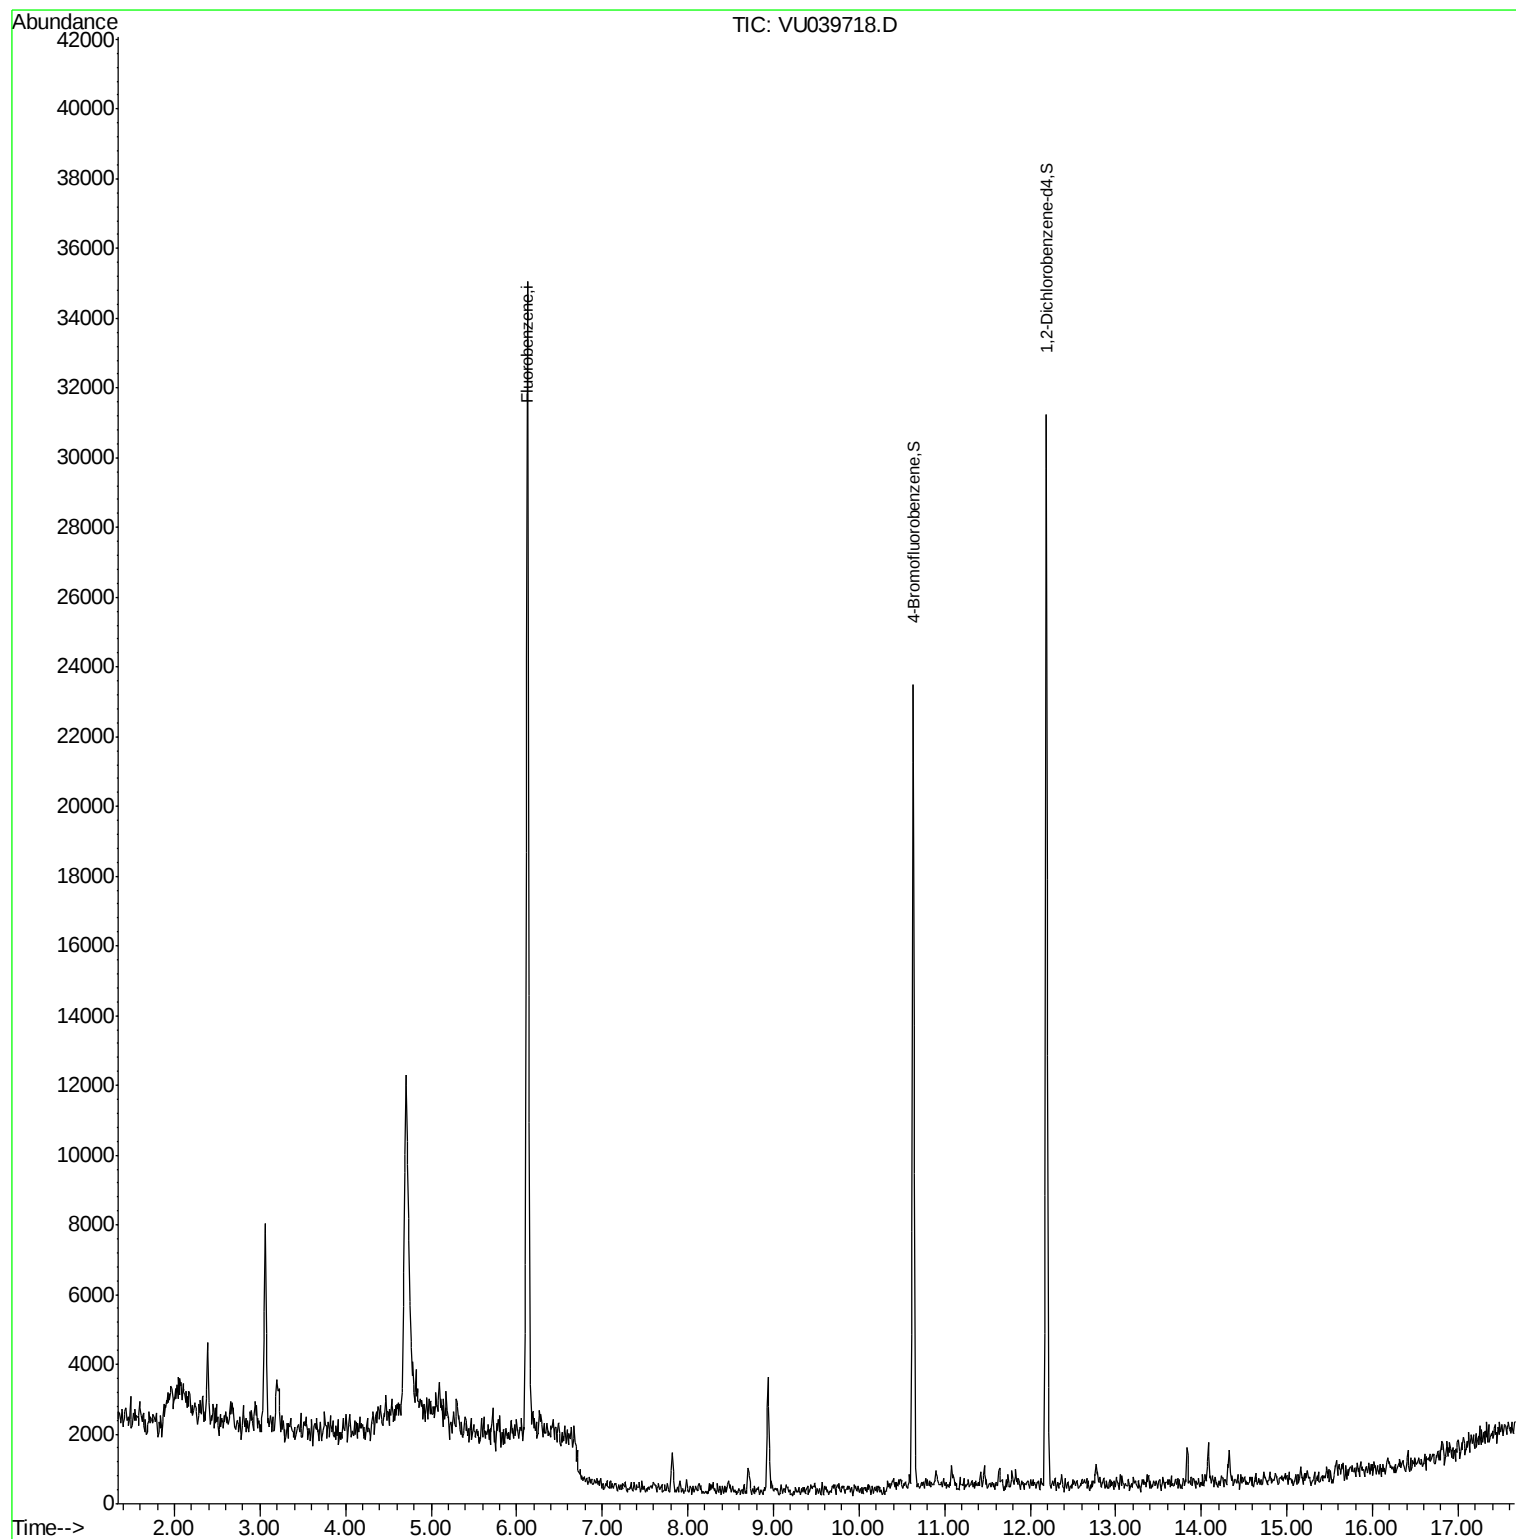

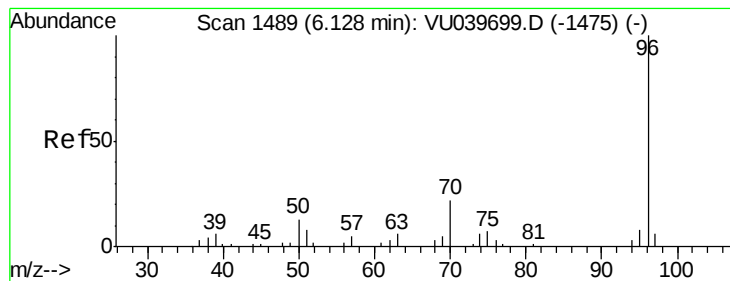

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.13 min Scan# 1489

Delta R.T. -0.00 min

Lab File: VU039718.D

Acq: 30 Jul 2020 12:19

Instrument :

MSVOA_U

ClientSampleId :

VU0730WBL01

Tot Ion: 96 Resp: 26489


Ion Ratio Lower Upper

96 100




70 22.5 16.3 24.5

95 9.0 6.8 10.2

97 6.5 0.0 0.0#

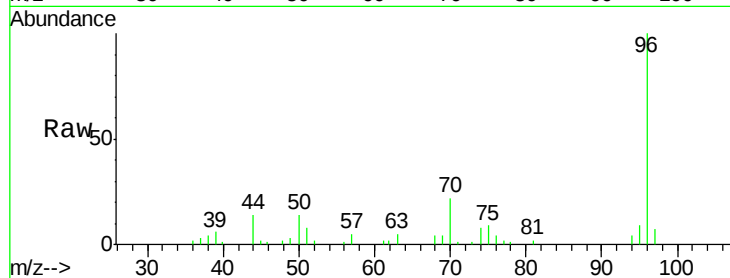

Abundance Ion 96.00 (95.70 to 96.70): VU039718.D (-1178) (-)

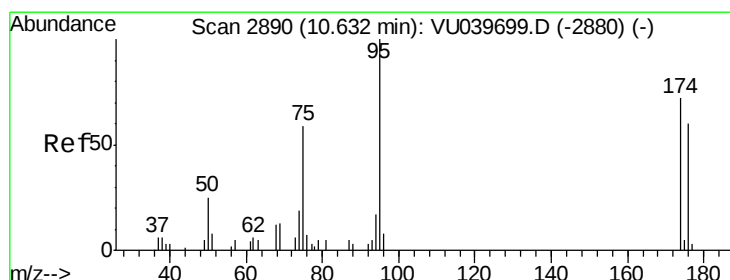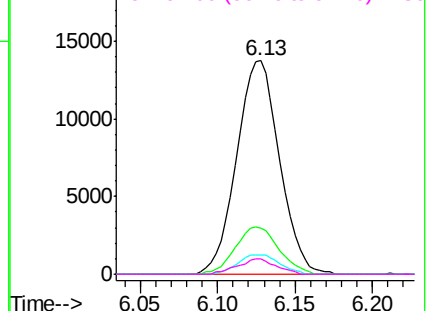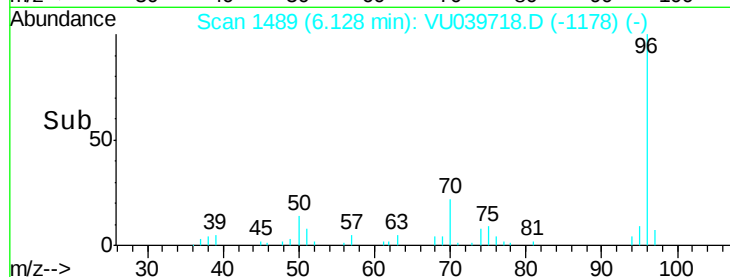

#57

4-Bromofluorobenzene

Concen: 0.733 ug/l

RT: 10.63 min Scan# 2890

Delta R.T. -0.00 min

Lab File: VU039718.D

Acq: 30 Jul 2020 12:19


Tgt Ion: 95 Resp: 7587

Ion Ratio Lower Upper



95 100


174 67.6 57.0 85.4

176 62.7 50.2 75.2

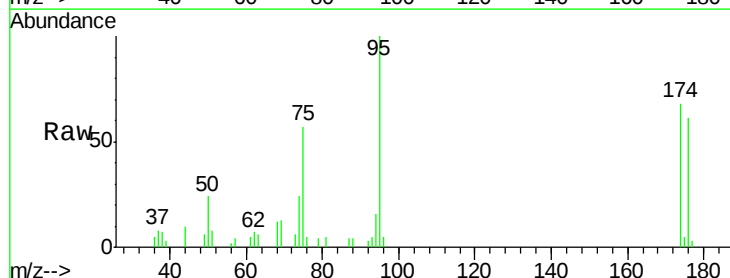

Abundance Ion 95.00 (94.70 to 95.70): VU039718.D (-2579) (-)

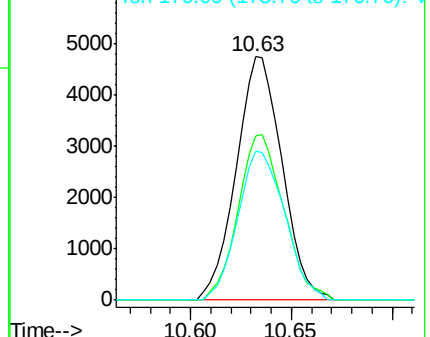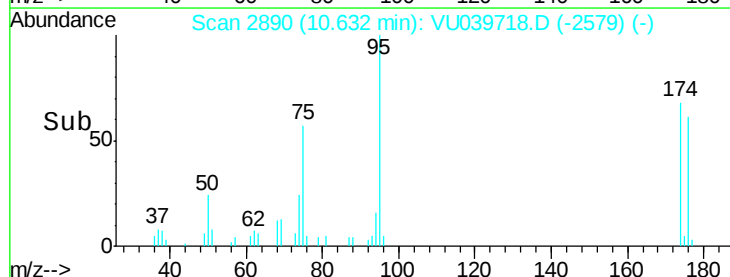

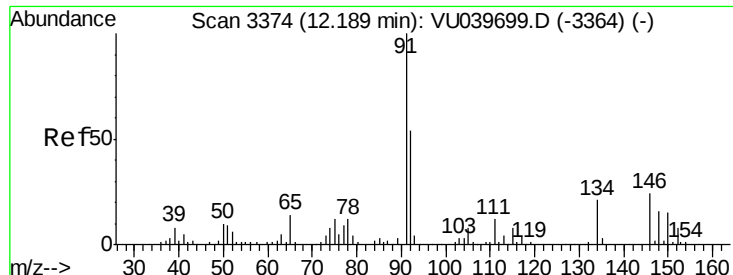

#68

1,2-Dichlorobenzene-d4

Concen: 0.713 ug/l

RT: 12.19 min Scan# 3374

Delta R.T. -0.00 min

Lab File: VU039718.D

Acq: 30 Jul 2020 12:19

Instrument :

MSVOA_U

ClientSampleId :

VU0730WBL01


Tot Ion:152 Resp: 7224

Ion Ratio Lower Upper

152 100

115 68.1 0.0 302.4

150 162.4 0.0 645.8

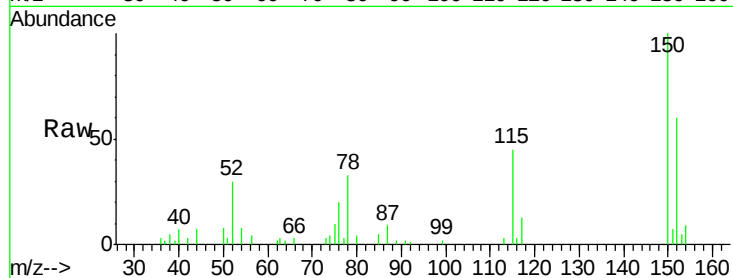

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

