

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073024\
 Data File : VU060271.D
 Acq On : 30 Jul 2024 18:56
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U073024DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.576	396	400	405	rVB4	944	793	1.02%	0.328%
2	2.631	412	417	420	rBV4	812	870	1.12%	0.359%
3	3.039	533	544	561	rVB2	12124	23888	30.87%	9.868%
4	3.917	812	817	820	rBV5	916	933	1.21%	0.385%
5	3.956	825	829	832	rBV3	1197	1107	1.43%	0.457%
6	4.351	949	952	954	rBV2	1183	834	1.08%	0.345%
7	4.660	1042	1048	1049	rBV3	1038	967	1.25%	0.399%
8	5.255	1226	1233	1237	rBV2	1159	1510	1.95%	0.624%
9	6.107	1485	1498	1514	rBV	40110	77375	100.00%	31.963%
10	6.538	1625	1632	1640	rVB3	738	1100	1.42%	0.454%
11	8.701	2299	2305	2308	rBV2	837	841	1.09%	0.347%
12	9.415	2519	2527	2531	rBV3	779	932	1.20%	0.385%
13	9.698	2609	2615	2622	rBV4	917	1013	1.31%	0.418%
14	10.631	2896	2905	2921	rVB2	24773	40497	52.34%	16.729%
15	10.907	2986	2991	2995	rBV2	792	833	1.08%	0.344%
16	11.107	3040	3053	3059	rVB3	567	1086	1.40%	0.449%
17	11.753	3247	3254	3259	rVB4	952	1084	1.40%	0.448%
18	11.824	3259	3276	3278	rBV7	1439	2740	3.54%	1.132%
19	11.840	3278	3281	3288	rVB4	1038	1034	1.34%	0.427%
20	12.190	3379	3390	3408	rBV2	34776	61809	79.88%	25.533%
21	13.846	3897	3905	3911	rBV6	2401	3428	4.43%	1.416%
22	13.930	3925	3931	3936	rVB3	623	795	1.03%	0.328%
23	14.090	3974	3981	3994	rBV2	4758	7597	9.82%	3.138%
24	14.325	4046	4054	4067	rBV7	3602	6389	8.26%	2.639%
25	14.656	4150	4157	4166	rVB5	604	801	1.04%	0.331%
26	16.296	4662	4667	4670	rBV5	783	889	1.15%	0.367%
27	16.466	4716	4720	4727	rBV3	825	933	1.21%	0.385%




Sum of corrected areas: 242078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073024\
Data File : VU060271.D
Acq On : 30 Jul 2024 18:56
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U073024DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

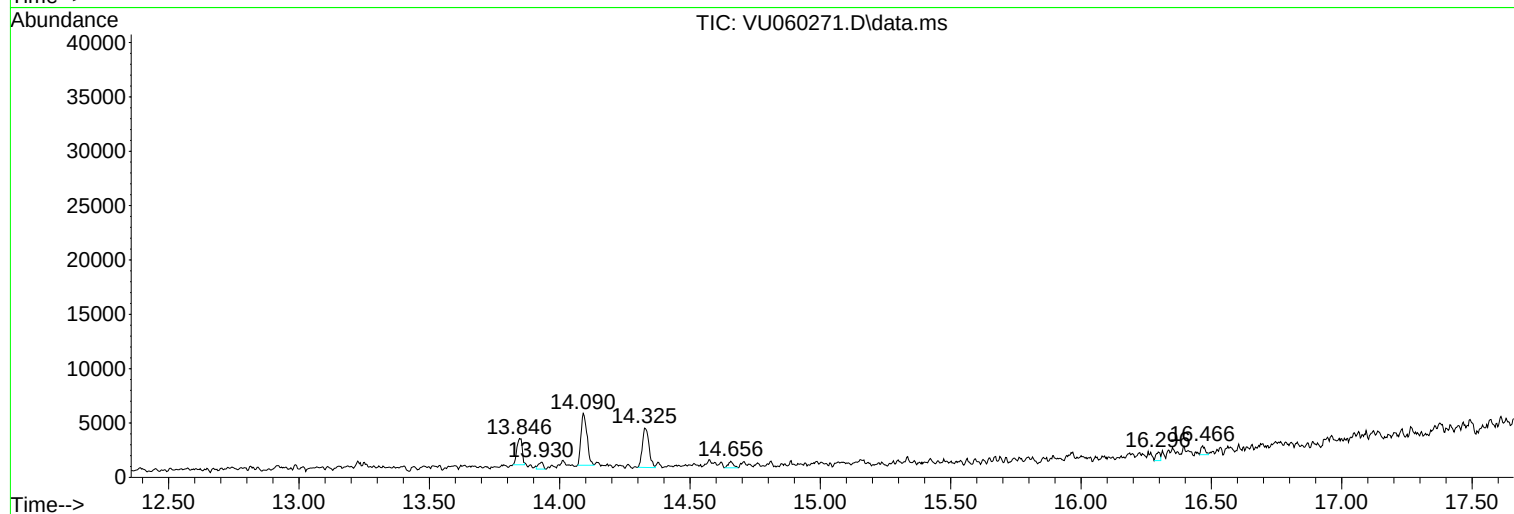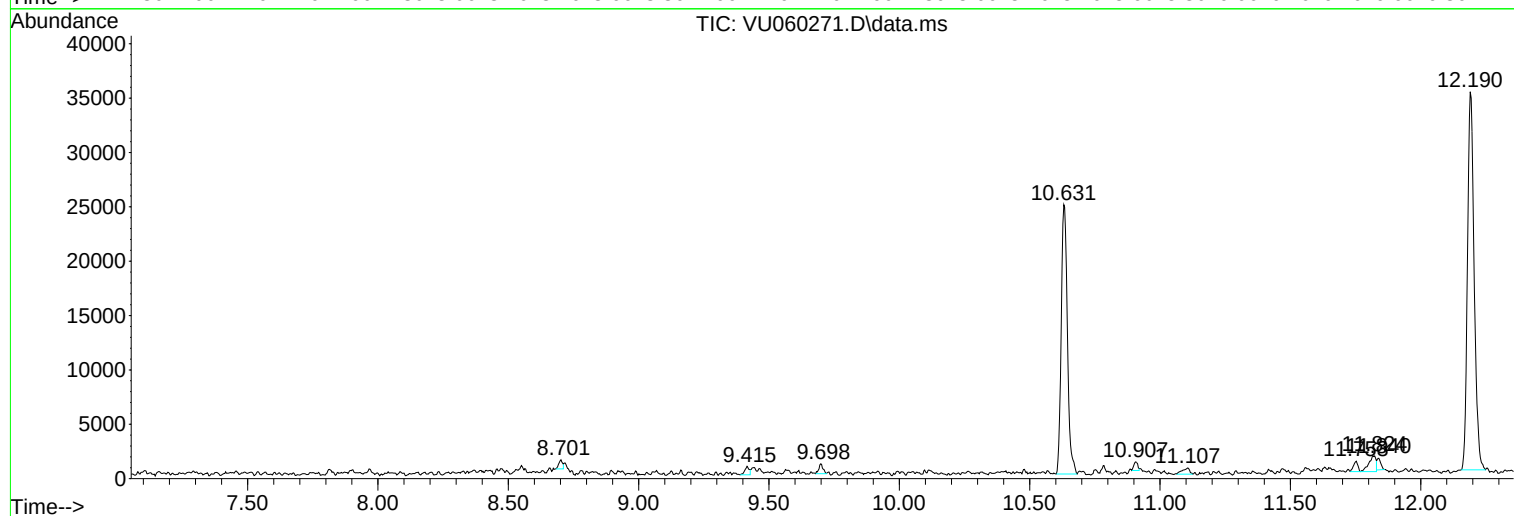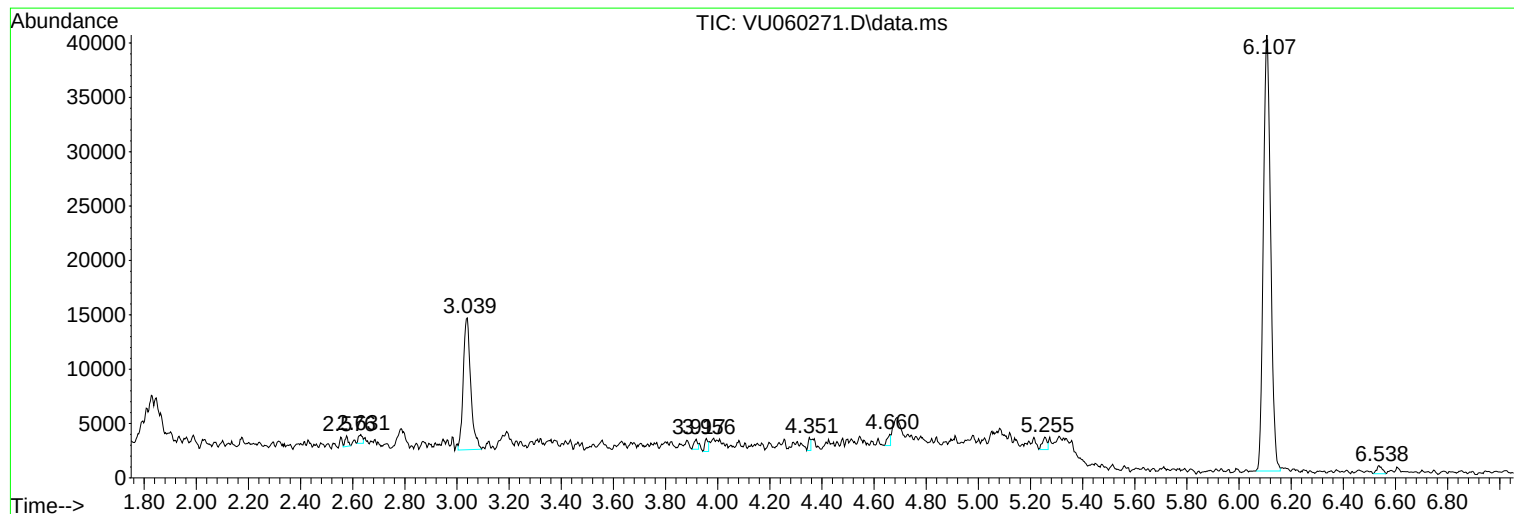

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073024\
Data File : VU060271.D
Acq On : 30 Jul 2024 18:56
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U073024DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073024\
Data File : VU060271.D
Acq On : 30 Jul 2024 18:56
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U073024DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------