


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073024\
Data File : VU060264.D
Acq On : 30 Jul 2024 13:59
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U073024DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Jul 31 04:49:33 2024

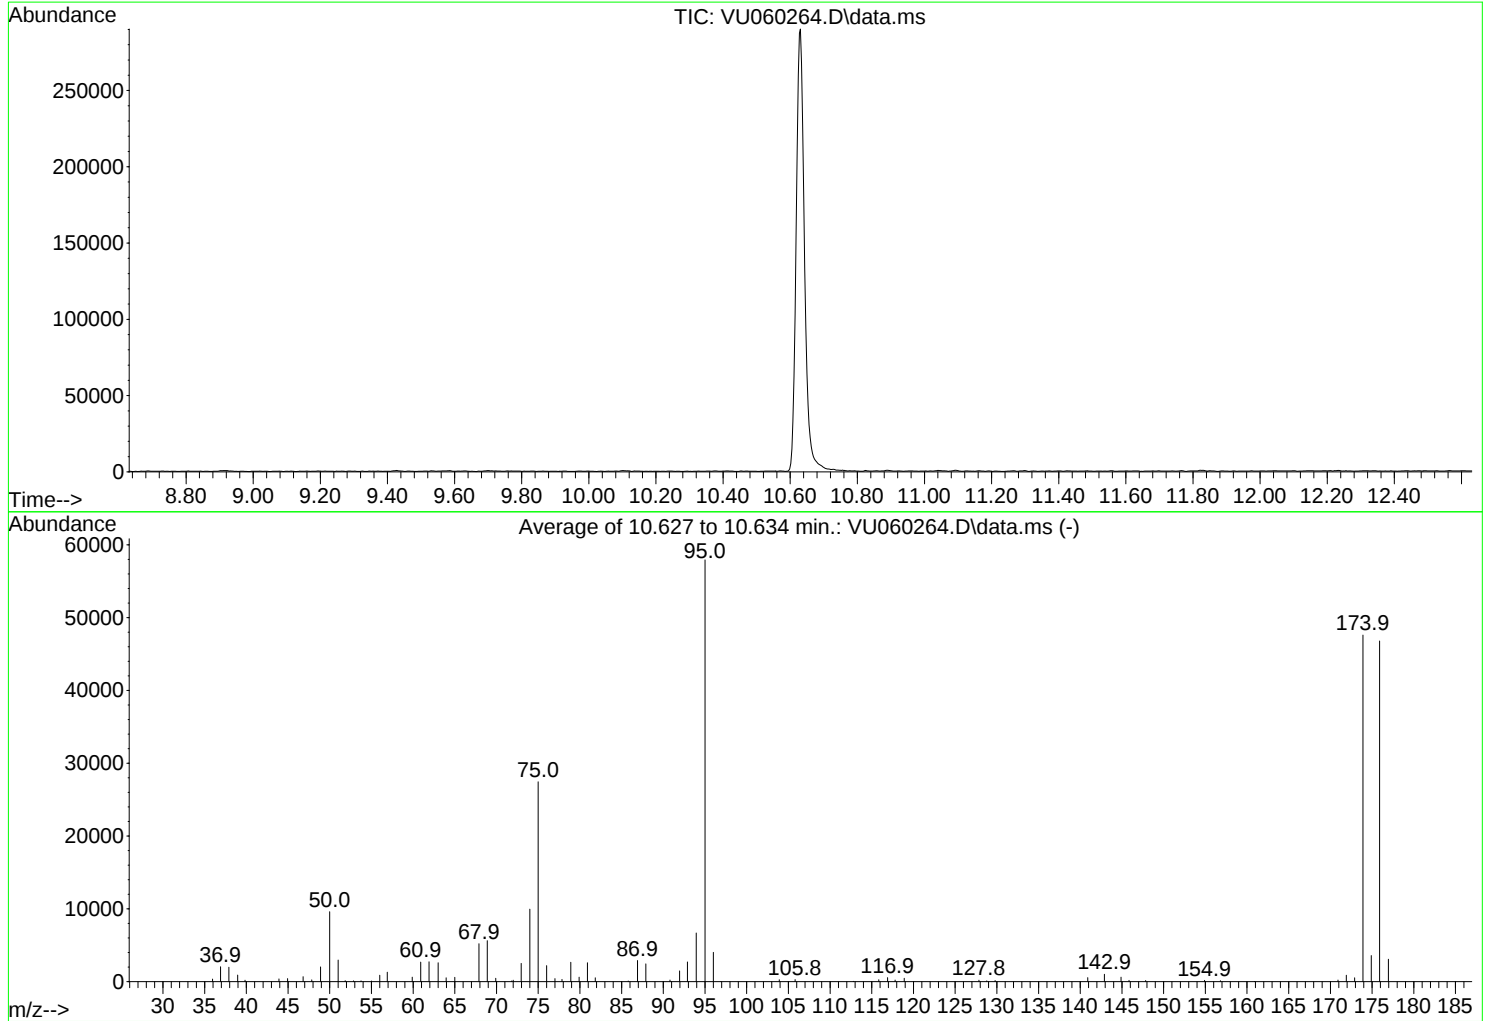

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9599	PASS
75	95	30	60	47.4	27448	PASS
95	95	100	100	100.0	57936	PASS
96	95	5	9	7.0	4030	PASS
173	174	0.00	2	1.1	528	PASS
174	95	50	100	82.2	47597	PASS
175	174	5	9	7.5	3586	PASS
176	174	95	101	98.3	46787	PASS
177	176	5	9	6.6	3081	PASS