


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU073118\
Data File : VU025730.D
Acq On : 31 Jul 2018 07:41
Operator : MD/SY
Sample : BFB51
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis
Last Update : Fri Jul 27 18:17:45 2018

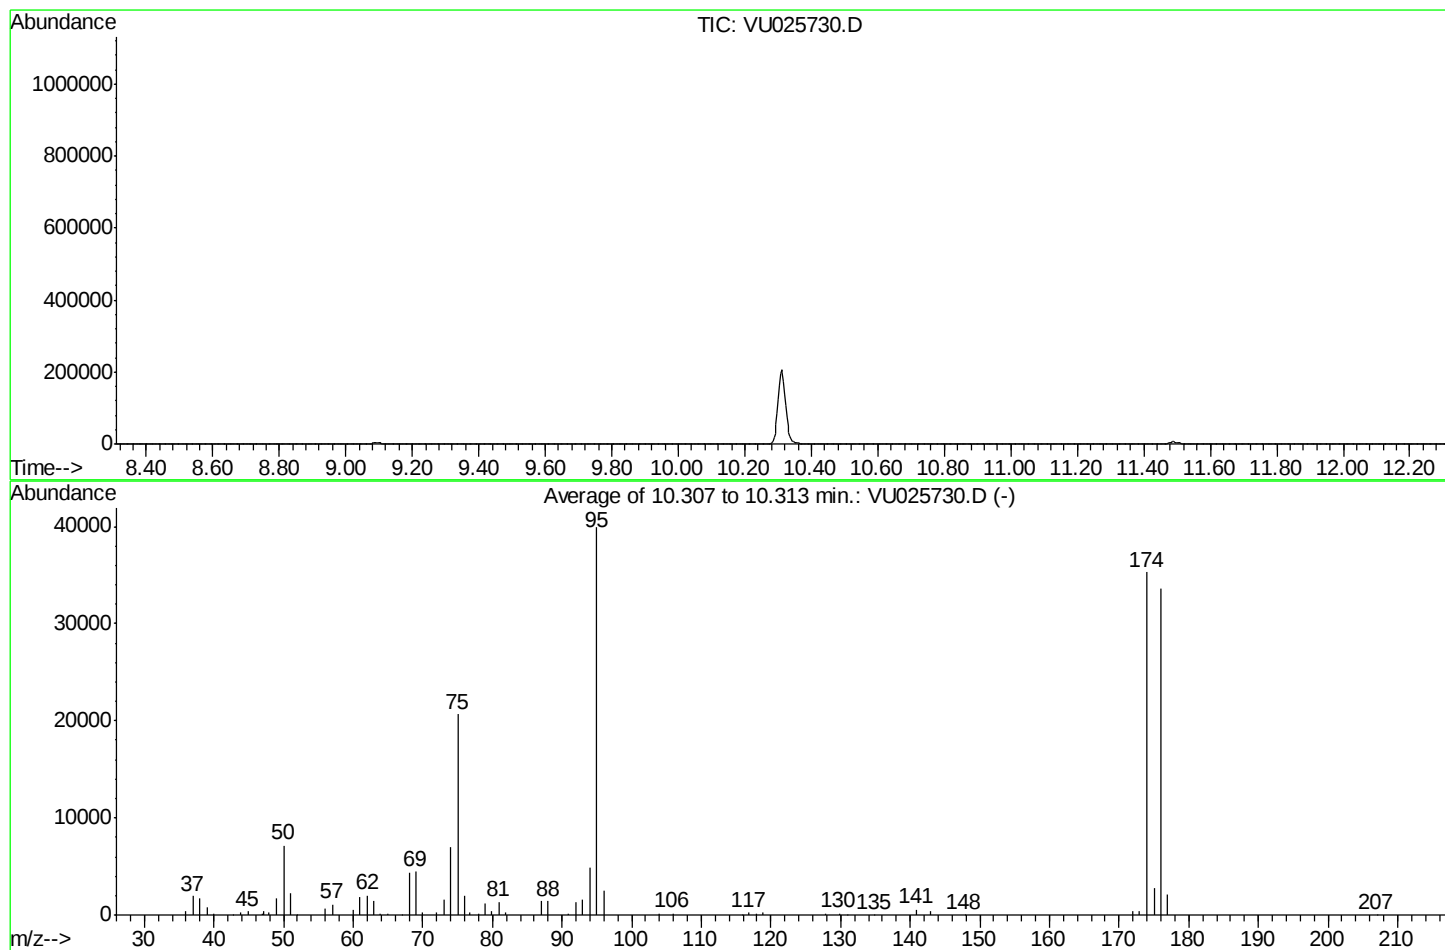

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7141	PASS
75	95	30	80	51.7	20642	PASS
95	95	100	100	100.0	39914	PASS
96	95	5	9	6.3	2512	PASS
173	174	0.00	2	1.1	392	PASS
174	95	50	120	88.4	35277	PASS
175	174	5	9	7.8	2752	PASS
176	174	95	101	95.3	33626	PASS
177	176	5	9	6.2	2085	PASS

m/z	Abundance
43.90	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	345.0
37.00	2003.0
38.00	1719.0
39.00	736.0
40.00	173.0
43.90	545.0
44.90	381.0
46.90	382.0
48.00	218.0
49.00	1604.0
50.00	7018.0
51.10	2158.0
56.00	678.0
57.00	1093.0
60.00	453.0
61.00	1914.0
62.10	1961.0
63.00	1417.0
64.00	184.0
64.90	183.0
68.00	4263.0
69.00	4401.0
69.90	219.0
71.90	243.0
73.00	1703.0
74.00	6612.0
75.00	20040.0
76.00	1744.0
76.80	247.0
78.10	121.0
78.90	1294.0
79.90	351.0
80.90	1370.0
81.90	338.0
87.00	1323.0
88.00	1493.0
90.90	134.0
92.00	1477.0
93.00	1619.0
94.00	4597.0
95.00	39056.0
96.00	2609.0
104.00	129.0
106.00	175.0
115.80	115.0
116.90	236.0
117.80	163.0
118.80	253.0
127.80	147.0
129.80	112.0
134.90	112.0
140.90	499.0
142.80	409.0
171.90	400.0
173.00	410.0
174.00	33512.0
175.00	2832.0
176.00	31808.0
176.90	2056.0
207.00	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	393.0
37.00	2011.0
38.00	1847.0
39.00	800.0
40.00	135.0
42.80	107.0
44.00	546.0
44.90	421.0
47.10	497.0
47.90	248.0
49.00	1806.0
50.00	7368.0
51.10	2306.0
56.00	669.0
57.00	1183.0
60.00	467.0
61.00	1953.0
62.10	2079.0
63.00	1546.0
64.00	193.0
64.90	194.0
66.90	100.0
68.00	4495.0
69.00	4579.0
69.90	262.0
72.00	291.0
73.00	1667.0
74.00	7192.0
75.00	21496.0
76.00	2022.0
76.80	289.0
77.90	133.0
78.90	1299.0
79.80	346.0
80.90	1409.0
81.90	297.0
86.90	1433.0
88.00	1504.0
90.90	144.0
92.00	1430.0
93.00	1685.0
94.00	4990.0
95.00	41240.0
96.00	2551.0
103.90	136.0
105.90	198.0
116.80	254.0
117.80	165.0
118.90	229.0
127.90	143.0
129.90	128.0
130.90	113.0
140.90	631.0
142.80	449.0
171.90	436.0
173.00	397.0
174.00	36712.0
175.00	2870.0
176.00	34904.0
177.00	2180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	345.0
37.00	1742.0
38.00	1718.0
39.00	720.0
39.80	141.0
44.00	545.0
44.90	369.0
47.10	518.0
47.90	282.0
49.00	1762.0
50.00	7037.0
51.00	2209.0
52.00	108.0
56.00	610.0
57.00	1090.0
60.10	485.0
61.00	1803.0
62.00	2047.0
63.00	1502.0
63.90	181.0
64.90	181.0
68.00	4293.0
69.00	4285.0
69.90	268.0
72.00	310.0
73.00	1485.0
74.00	7165.0
75.00	20392.0
76.00	2001.0
76.80	262.0
77.90	131.0
78.90	1167.0
79.80	311.0
80.90	1299.0
81.90	246.0
86.90	1542.0
88.00	1350.0
90.90	170.0
92.00	1135.0
93.00	1603.0
94.00	4951.0
95.00	39448.0
96.00	2376.0
103.80	169.0
105.80	220.0
116.80	242.0
117.90	178.0
118.90	208.0
127.90	105.0
129.90	164.0
130.90	100.0
140.90	654.0
142.90	491.0
147.80	113.0
171.90	369.0
172.80	369.0
174.00	35608.0
175.00	2554.0
176.00	34168.0
177.00	2021.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51