
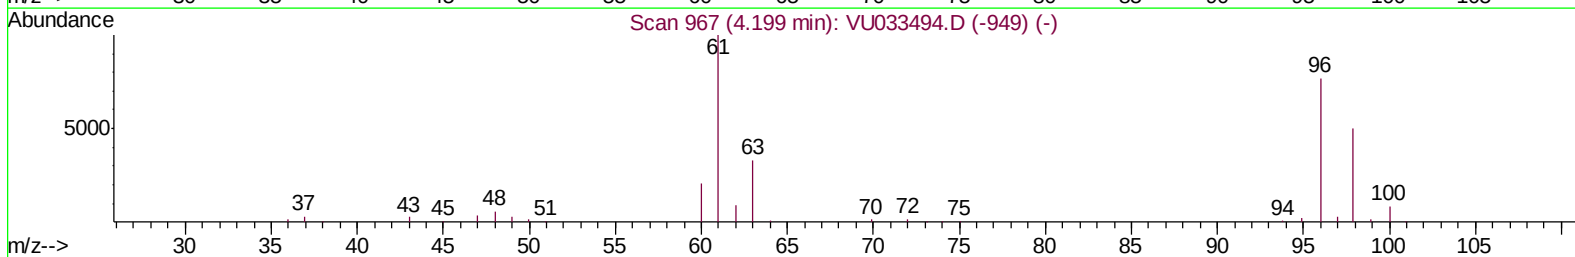
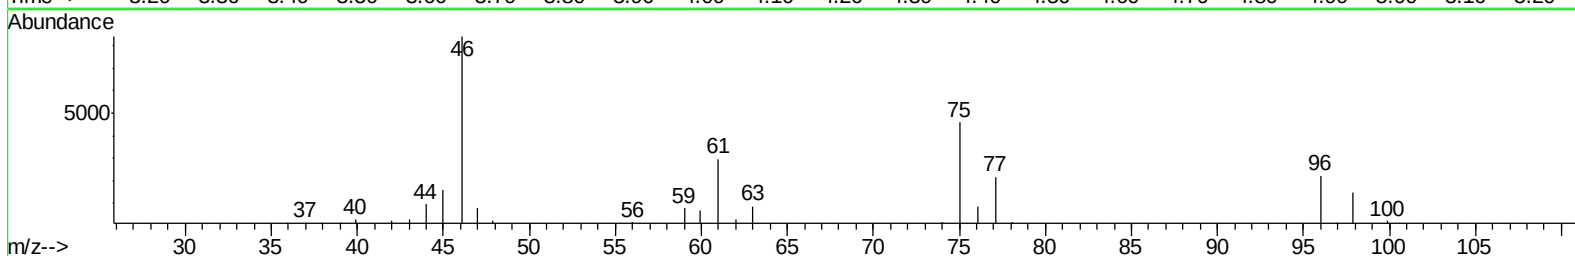


Data File : VU033502.D
Acq On : 30 Jul 2019 19:12
Operator : JC/SP
Sample : MDL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jul 31 08:08:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 08:02:52 2019
Response via : Initial Calibration

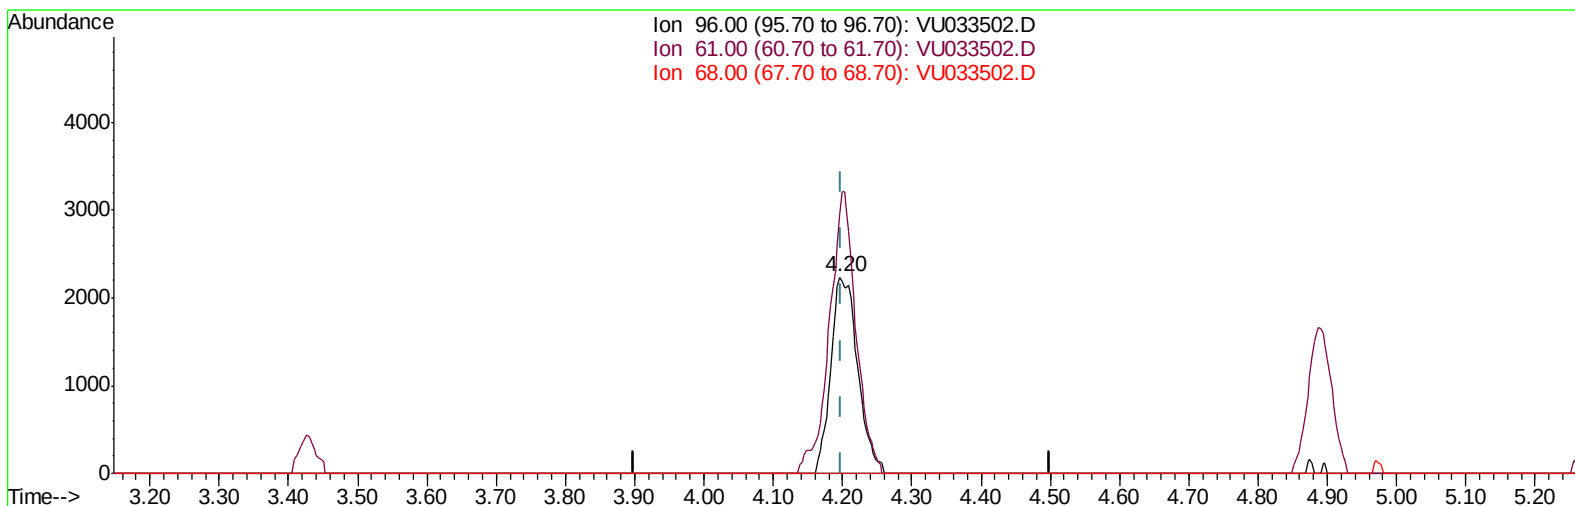

TIC: VU033502.D

(20) cis-1,2-Dichloroethene (T)

4.196min (-0.003) 2.44ug/L m

response 5989

Ion	Exp%	Act%
96.00	100	100
61.00	130.50	132.11
68.00	0.00	0.00
0.00	0.00	0.00