
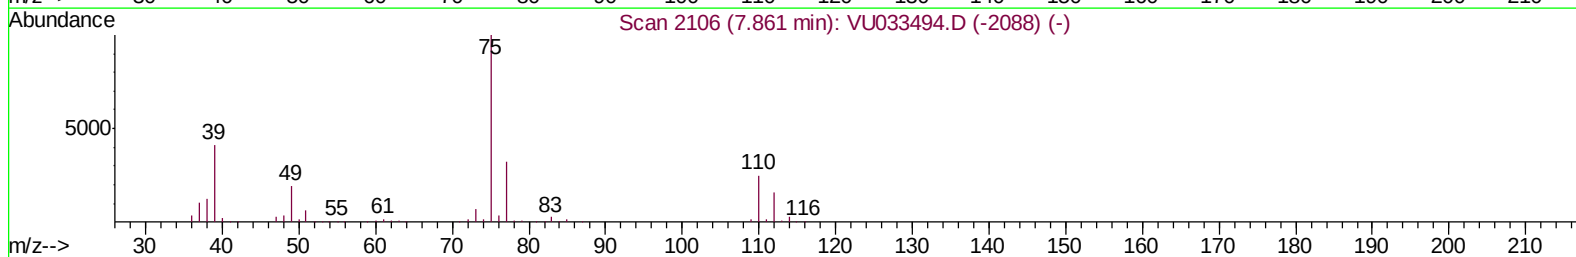
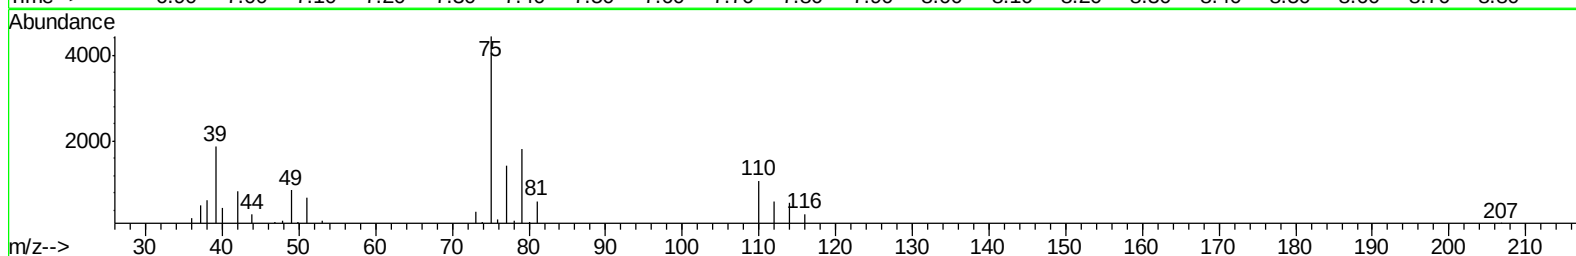


Data File : VU033503.D
Acq On : 30 Jul 2019 19:34
Operator : JC/SP
Sample : MDL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jul 31 08:09:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 08:02:52 2019
Response via : Initial Calibration

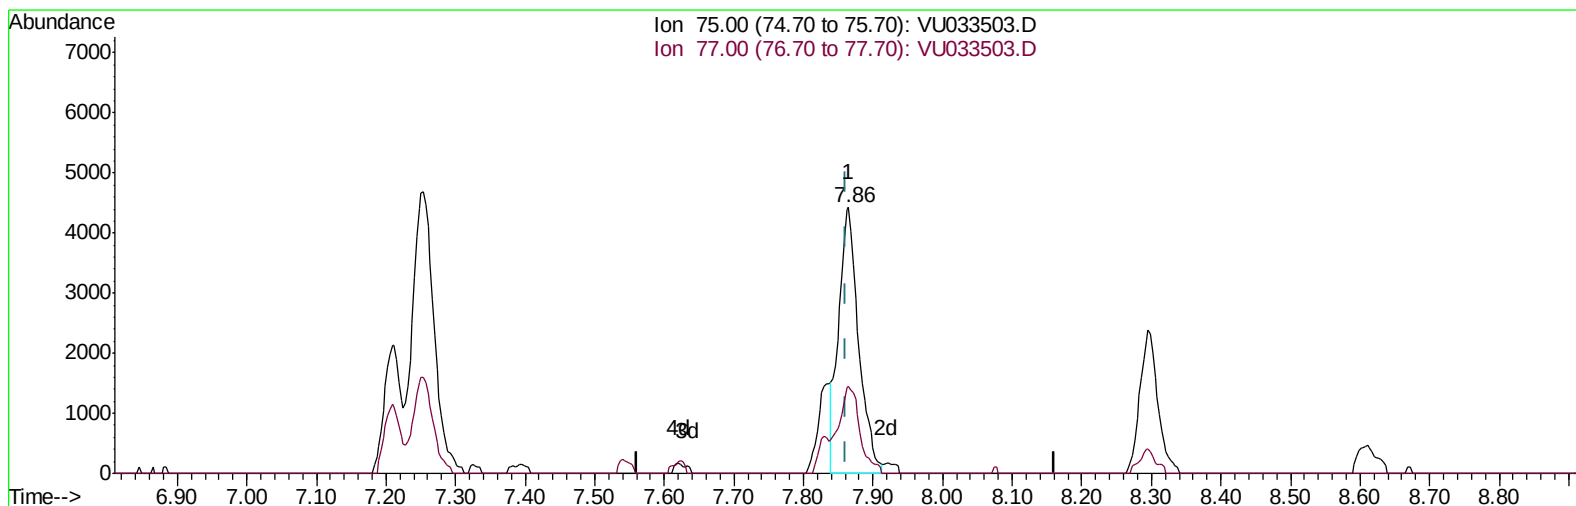

TIC: VU033503.D

(44) trans-1,3-Dichloropropene (T)

7.865min (+0.003) 2.42ug/L m

response 8783

Ion	Exp%	Act%
75.00	100	100
77.00	32.40	32.52
0.00	0.00	0.00
0.00	0.00	0.00