
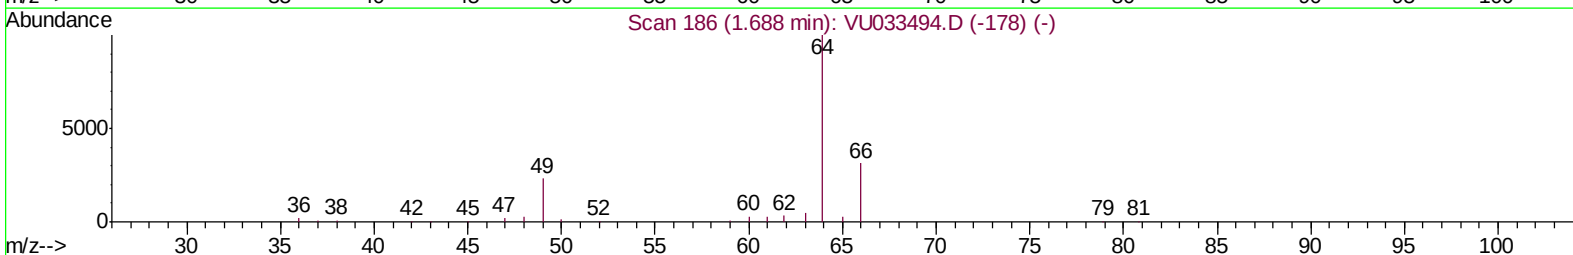
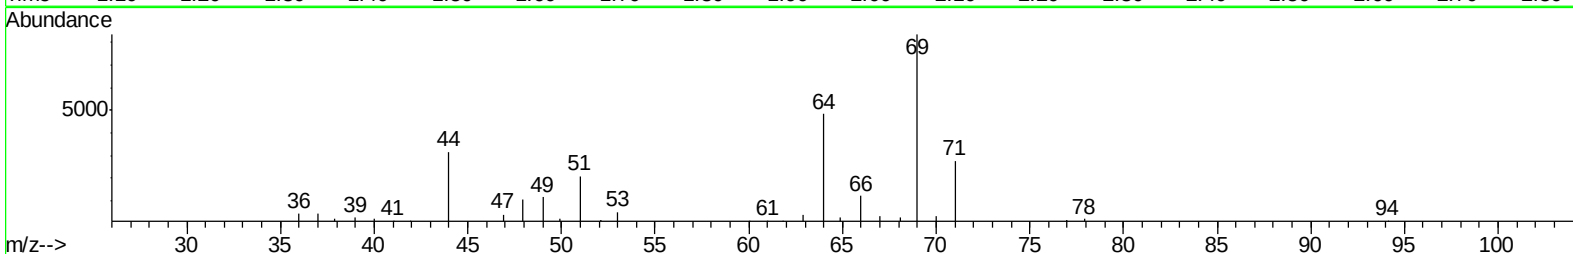


Data File : VU033504.D
Acq On : 30 Jul 2019 19:57
Operator : JC/SP
Sample : MDL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jul 31 08:09:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 08:02:52 2019
Response via : Initial Calibration

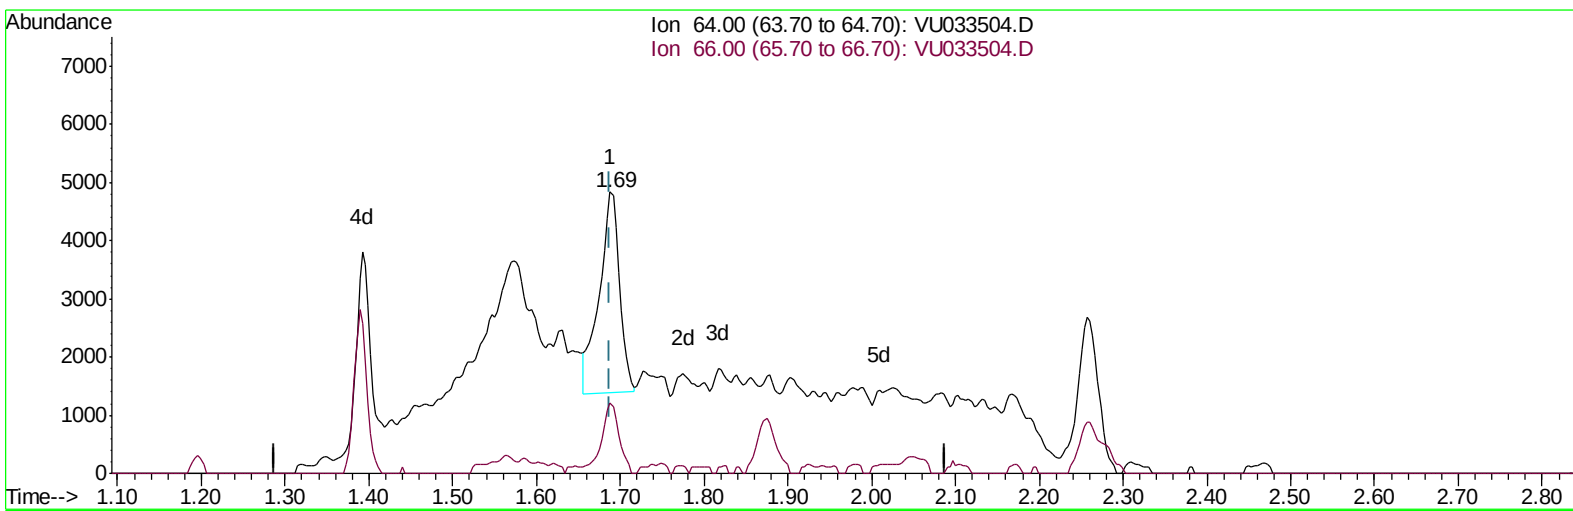

TIC: VU033504.D

(8) Chloroethane (T)

1.688min (+0.000) 3.03ug/L m

response 5703

Ion	Exp%	Act%
64.00	100	100
66.00	30.20	25.02
0.00	0.00	0.00
0.00	0.00	0.00