
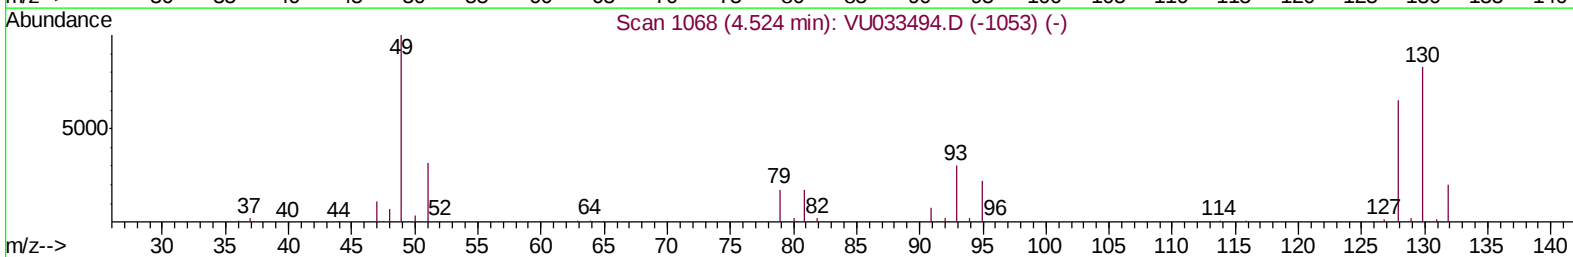
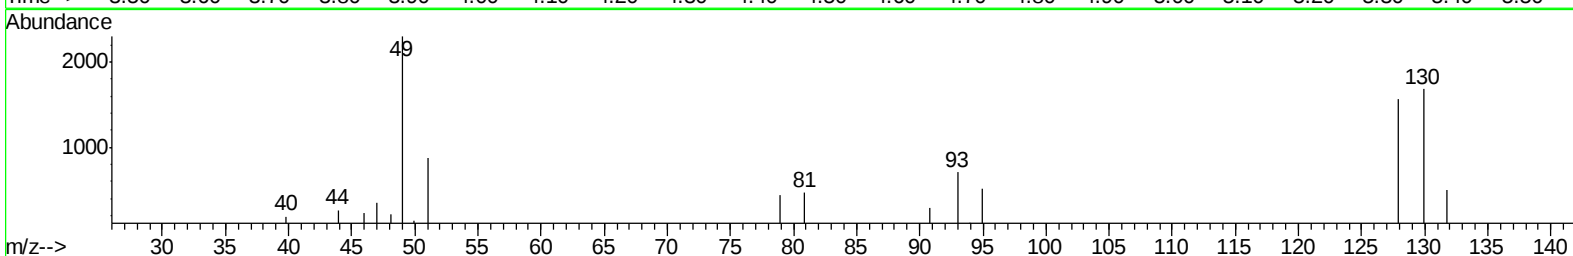


Data File : VU033506.D
Acq On : 30 Jul 2019 20:43
Operator : JC/SP
Sample : MDL06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jul 31 08:10:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 08:02:52 2019
Response via : Initial Calibration

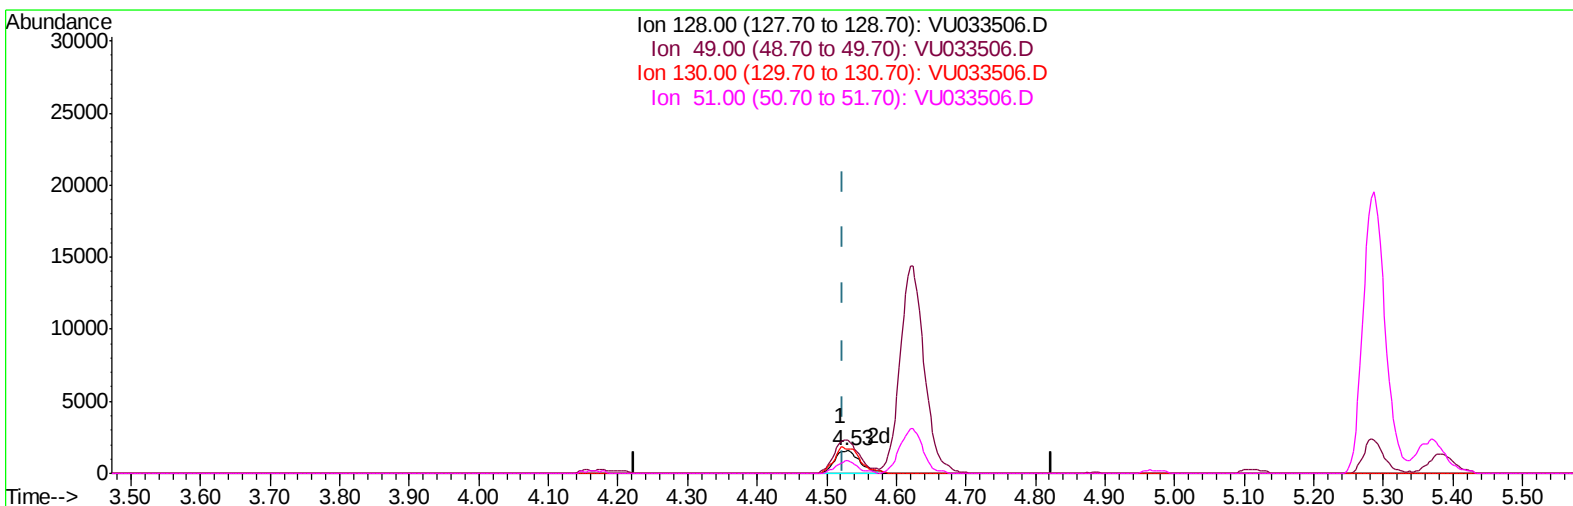

TIC: VU033506.D

(23) Bromochloromethane (T)

4.530min (+0.006) 3.11ug/L m

response 3918

Ion	Exp%	Act%
128.00	100	100
49.00	154.80	147.63
130.00	128.10	108.09
51.00	48.60	55.84