

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033509.D
 Acq On : 30 Jul 2019 22:38
 Operator : JC/SP
 Sample : K4103-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9D7

Quant Time: Jul 31 08:36:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 31 08:02:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	302486	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	300876	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	139591	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	105946	48.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.34%
7) Chloroethane-d5	1.67	69	106512	56.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.90%
11) 1,1-Dichloroethene-d2	2.26	63	144008	36.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.16%
21) 2-Butanone-d5	4.16	46	156630	107.53	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.53%
24) Chloroform-d	4.62	84	183147	49.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.36%
26) 1,2-Dichloroethane-d4	5.29	65	122959	52.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.34%
32) Benzene-d6	5.32	84	379847	50.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.86%
36) 1,2-Dichloropropane-d6	6.31	67	120445	51.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.02%
41) Toluene-d8	7.55	98	339933	48.64	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.28%
43) trans-1,3-Dichloropropene-	7.83	79	56306	48.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.10%
47) 2-Hexanone-d5	8.30	63	114767	103.39	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.39%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	178381	49.48	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.96%
64) 1,2-Dichlorobenzene-d4	11.85	152	133177	52.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.20%


Target Compounds					Ovalue
20) cis-1,2-Dichloroethene	4.20	96	30374	13.186 ug/L	92
34) Trichloroethene	6.17	95	30514	13.327 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
Data File : VU033509.D
Acq On : 30 Jul 2019 22:38
Operator : JC/SP
Sample : K4103-03 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9D7

Quant Time: Jul 31 08:36:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 08:02:52 2019
Response via : Initial Calibration

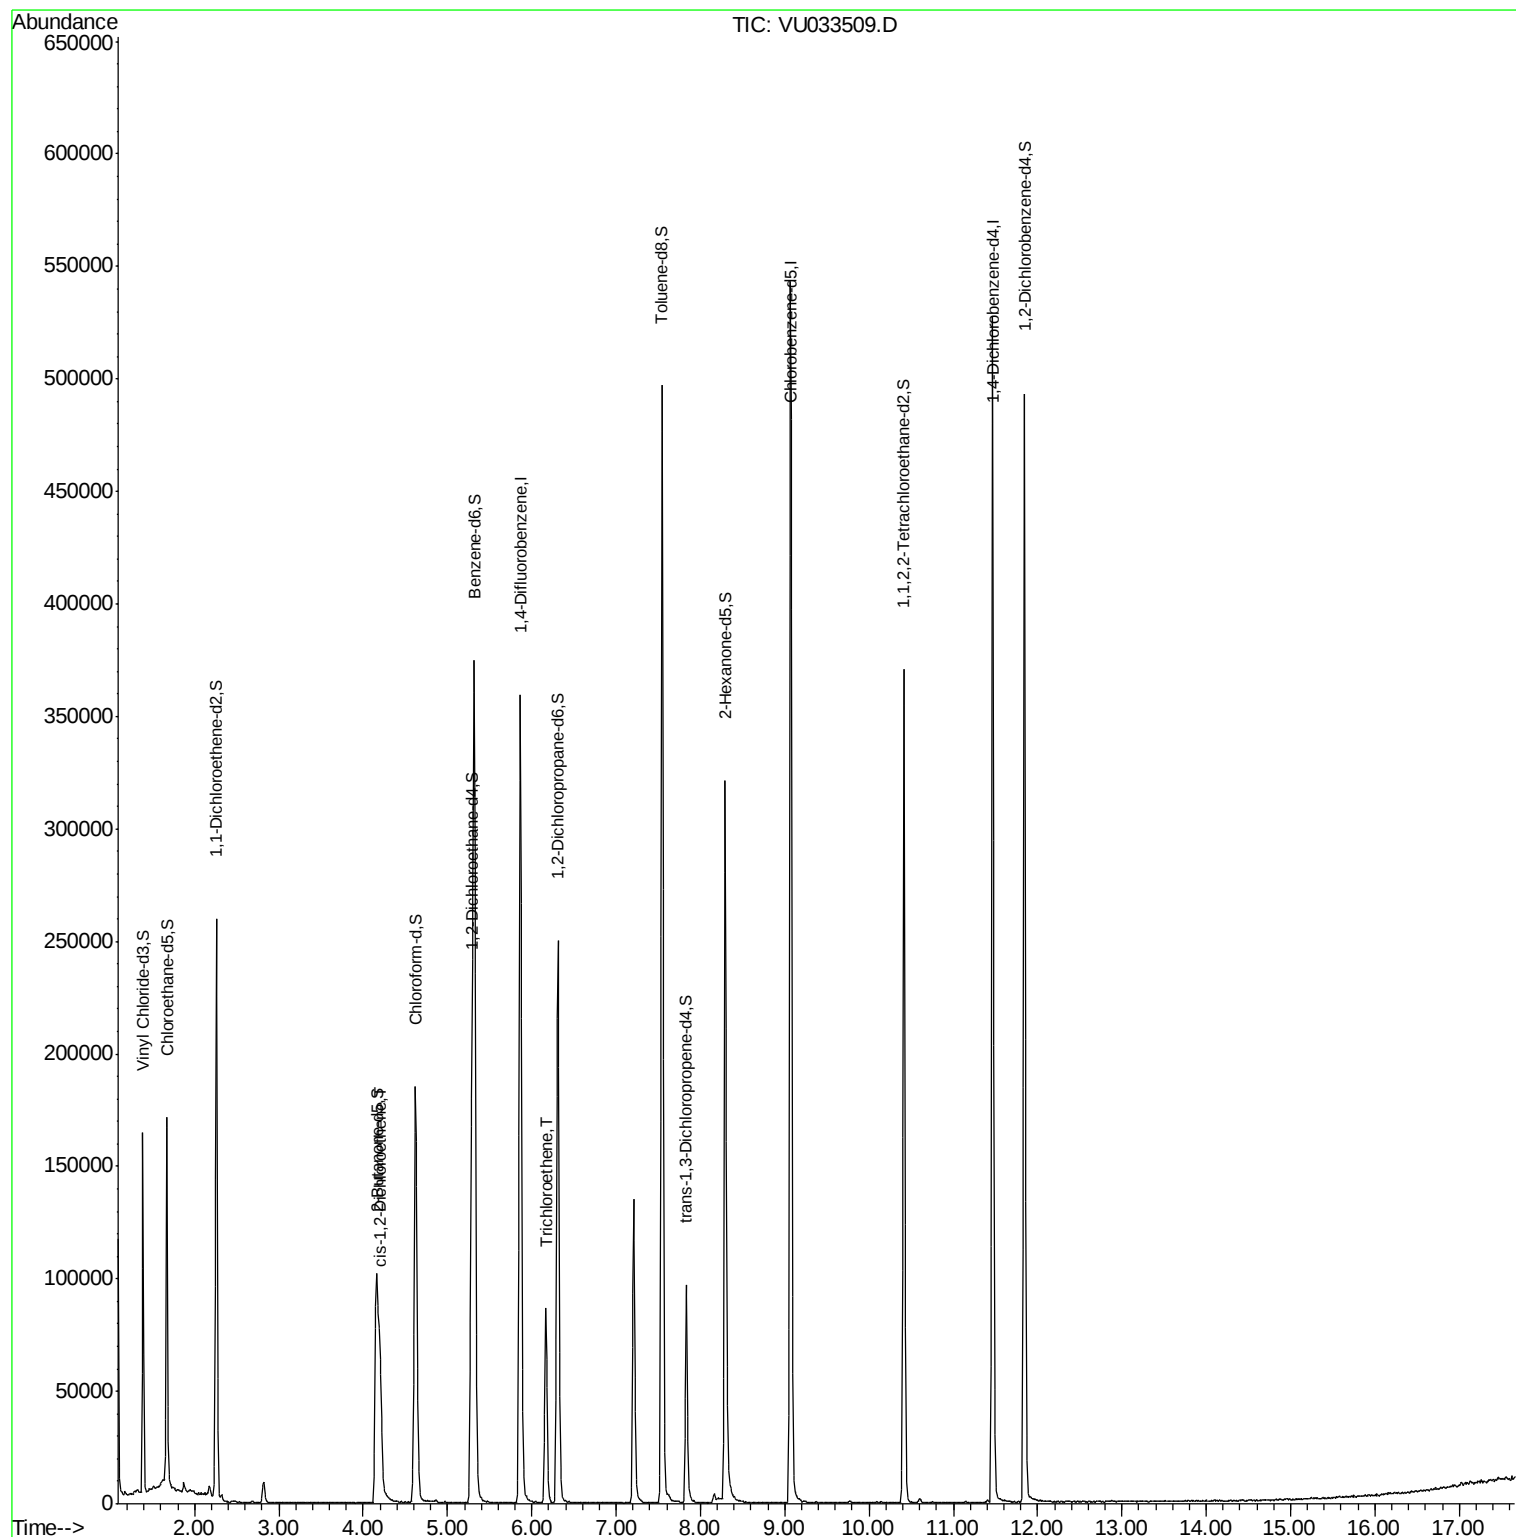

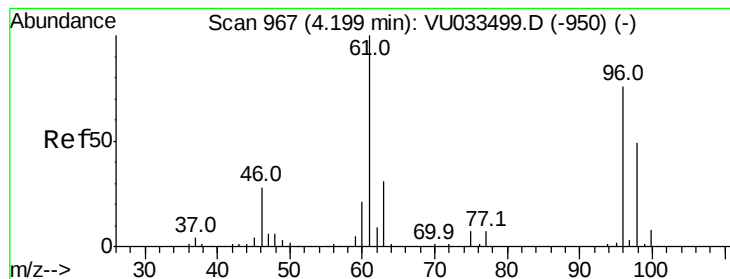


#20




cis-1,2-Dichloroethene
 Concen: 13.186 ug/L
 RT: 4.20 min Scan# 968
 Delta R.T. 0.00 min
 Lab File: VU033509.D
 Acq: 30 Jul 2019 22:38

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9D7

Tot Ion: 96 Resp: 30374
 Ion Ratio Lower Upper
 96 100
 61 120.8 91.3 169.6
 68 0.0 0.0 0.0

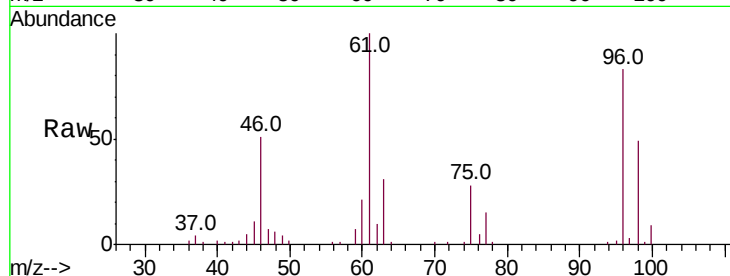


Abundance Ion 96.00 (95.70 to 96.70): VU0
 Ion 61.00 (60.70 to 61.70): VU0
 Ion 68.00 (67.70 to 68.70): VU0

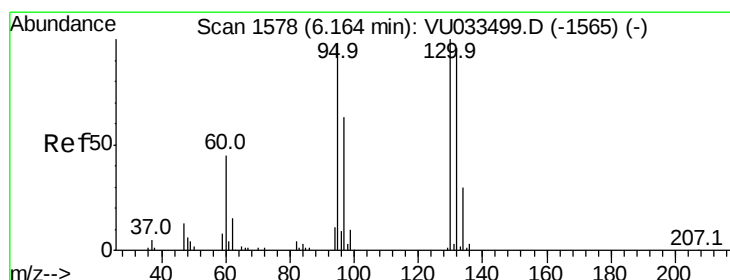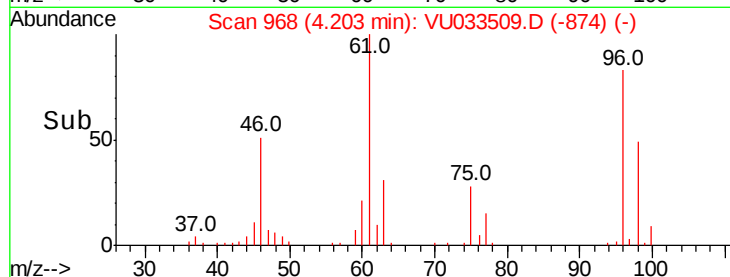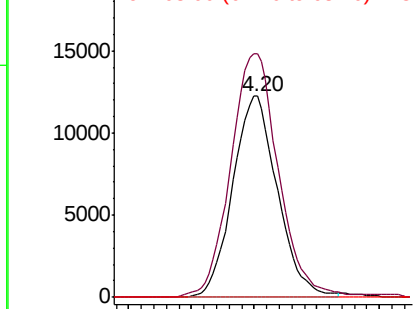

#34

Trichloroethene
 Concen: 13.327 ug/L
 RT: 6.17 min Scan# 1579
 Delta R.T. 0.00 min
 Lab File: VU033509.D
 Acq: 30 Jul 2019 22:38

Tgt Ion: 95 Resp: 30514
 Ion Ratio Lower Upper
 95 100
 97 62.7 44.7 83.1
 132 98.4 66.8 124.0
 130 100.5 71.6 133.0

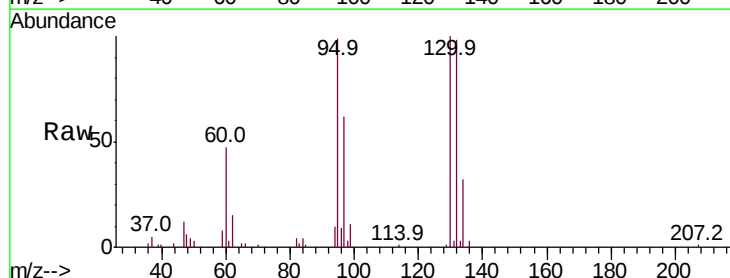

Abundance Ion 95.00 (94.70 to 95.70): VU0
 Ion 97.00 (96.70 to 97.70): VU0
 Ion 132.00 (131.70 to 132.70): V
 Ion 130.00 (129.70 to 130.70): V

