

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033497.D
 Acq On : 30 Jul 2019 16:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	86	93	106	rVB	180170	191609	16.35%	1.898%
2	1.672	174	181	199	rVB	161285	201023	17.15%	1.991%
3	2.257	353	363	377	rVB	277554	422960	36.09%	4.190%
4	2.463	418	427	440	rVB	10276	16712	1.43%	0.166%
5	2.685	489	496	507	rVB3	2230	3500	0.30%	0.035%
6	2.756	514	518	523	rVB4	348	318	0.03%	0.003%
7	2.820	525	538	552	rVV	6642	13968	1.19%	0.138%
8	2.968	571	584	598	rBV5	4827	9134	0.78%	0.090%
9	3.360	702	706	710	rBV4	253	311	0.03%	0.003%
10	3.736	818	823	824	rBV	391	269	0.02%	0.003%
11	3.955	887	891	897	rBV2	395	520	0.04%	0.005%
12	3.984	897	900	905	rVB2	324	255	0.02%	0.003%
13	4.026	911	913	918	rBV2	359	306	0.03%	0.003%
14	4.048	918	920	928	rVB3	318	326	0.03%	0.003%
15	4.164	941	956	987	rBV2	99697	313865	26.78%	3.109%
16	4.495	1056	1059	1064	rVV4	334	322	0.03%	0.003%
17	4.524	1064	1068	1075	rVB5	1098	1177	0.10%	0.012%
18	4.620	1081	1098	1122	rBV2	194099	461845	39.41%	4.575%
19	4.971	1197	1207	1217	rVB7	2339	4967	0.42%	0.049%
20	5.116	1249	1252	1258	rVB4	540	415	0.04%	0.004%
21	5.215	1278	1283	1289	rVB3	357	400	0.03%	0.004%
22	5.318	1290	1315	1349	rBV2	397825	1171861	100.00%	11.608%
23	5.453	1355	1357	1363	rVB4	572	454	0.04%	0.004%
24	5.617	1406	1408	1411	rVB2	360	235	0.02%	0.002%
25	5.733	1438	1444	1445	rBV3	337	301	0.03%	0.003%
26	5.807	1465	1467	1471	rVB	350	239	0.02%	0.002%
27	5.865	1471	1485	1509	rBV	409368	805110	68.70%	7.975%
28	6.170	1565	1580	1591	rBV10	4447	9762	0.83%	0.097%
29	6.228	1595	1598	1603	rVB3	402	311	0.03%	0.003%
30	6.309	1608	1623	1641	rBV	256677	516035	44.04%	5.112%
31	6.736	1752	1756	1757	rBV2	493	305	0.03%	0.003%
32	6.781	1764	1770	1772	rBV2	271	228	0.02%	0.002%
33	6.913	1806	1811	1817	rBV3	307	500	0.04%	0.005%
34	6.990	1830	1835	1839	rBV3	275	276	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033497.D
 Acq On : 30 Jul 2019 16:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

35	7.141	1877	1882	1885	rBV3	200	225	0.02%	0.002%
36	7.209	1889	1903	1934	rBV	149089	277033	23.64%	2.744%
37	7.392	1958	1960	1965	rVB2	710	398	0.03%	0.004%
38	7.450	1966	1978	1989	rBV3	5478	10202	0.87%	0.101%
39	7.546	1993	2008	2025	rBV	537888	941751	80.36%	9.329%
40	7.762	2073	2075	2082	rVB4	535	468	0.04%	0.005%
41	7.833	2085	2097	2123	rBV	105648	191769	16.36%	1.900%
42	8.016	2151	2154	2156	rVB2	467	280	0.02%	0.003%
43	8.054	2159	2166	2174	rVB4	1388	1995	0.17%	0.020%
44	8.161	2188	2199	2209	rBV2	14537	29759	2.54%	0.295%
45	8.296	2231	2241	2286	rVB	336692	607721	51.86%	6.020%
46	8.447	2286	2288	2290	rBV2	616	369	0.03%	0.004%
47	8.579	2321	2329	2330	rBV3	899	1177	0.10%	0.012%
48	8.604	2333	2337	2354	rVB5	3327	6247	0.53%	0.062%
49	8.807	2395	2400	2403	rBV3	354	270	0.02%	0.003%
50	8.855	2410	2415	2420	rBV3	265	324	0.03%	0.003%
51	8.887	2421	2425	2432	rVB2	420	493	0.04%	0.005%
52	8.952	2441	2445	2450	rVB3	537	481	0.04%	0.005%
53	9.013	2458	2464	2465	rBV	387	288	0.02%	0.003%
54	9.070	2469	2482	2511	rBV	607820	1018097	86.88%	10.085%
55	9.238	2525	2534	2545	rVB	6828	10111	0.86%	0.100%
56	9.308	2552	2556	2562	rVB4	391	316	0.03%	0.003%
57	9.360	2562	2572	2584	rBV2	7291	12325	1.05%	0.122%
58	9.572	2632	2638	2643	rBV3	466	548	0.05%	0.005%
59	9.617	2648	2652	2654	rVV2	452	302	0.03%	0.003%
60	9.633	2654	2657	2661	rVB4	503	395	0.03%	0.004%
61	9.662	2661	2666	2671	rBV2	450	481	0.04%	0.005%
62	9.775	2689	2701	2718	rVV5	9938	20786	1.77%	0.206%
63	9.878	2729	2733	2738	rBV3	369	334	0.03%	0.003%
64	9.935	2745	2751	2760	rBV7	1236	2047	0.17%	0.020%
65	10.045	2780	2785	2788	rBV3	577	497	0.04%	0.005%
66	10.080	2793	2796	2798	rBV	437	306	0.03%	0.003%
67	10.151	2806	2818	2827	rBV2	7632	11775	1.00%	0.117%
68	10.324	2866	2872	2876	rBV2	242	274	0.02%	0.003%
69	10.369	2880	2886	2887	rBV2	282	242	0.02%	0.002%
70	10.414	2887	2900	2916	rBV	381757	612531	52.27%	6.068%
71	10.527	2931	2935	2938	rBV3	367	285	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033497.D
 Acq On : 30 Jul 2019 16:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

72	10.598	2945	2957	2971	rVV5	6400	12817	1.09%	0.127%
73	10.672	2977	2980	2982	rBV3	319	232	0.02%	0.002%
74	10.759	2996	3007	3019	rBV2	8244	12778	1.09%	0.127%
75	10.858	3036	3038	3042	rBV2	317	248	0.02%	0.002%
76	10.932	3057	3061	3065	rBV3	274	258	0.02%	0.003%
77	10.955	3065	3068	3072	rBV3	302	227	0.02%	0.002%
78	11.048	3094	3097	3100	rBV2	534	408	0.03%	0.004%
79	11.086	3107	3109	3115	rVB3	354	322	0.03%	0.003%
80	11.135	3115	3124	3140	rVB	8928	13454	1.15%	0.133%
81	11.202	3142	3145	3151	rBV3	275	343	0.03%	0.003%
82	11.344	3184	3189	3191	rBV2	478	473	0.04%	0.005%
83	11.402	3196	3207	3216	rBV2	16862	25674	2.19%	0.254%
84	11.466	3216	3227	3251	rVV	628171	1024049	87.39%	10.144%
85	11.784	3324	3326	3332	rBV3	269	241	0.02%	0.002%
86	11.842	3332	3344	3369	rBV	548609	913557	77.96%	9.050%
87	12.151	3436	3440	3441	rBV2	573	336	0.03%	0.003%
88	12.205	3454	3457	3460	rVB3	364	233	0.02%	0.002%
89	12.385	3509	3513	3515	rBV2	463	350	0.03%	0.003%
90	12.421	3521	3524	3527	rBV2	513	397	0.03%	0.004%
91	12.469	3531	3539	3547	rVB3	2030	3189	0.27%	0.032%
92	12.646	3585	3594	3604	rBV7	3642	6844	0.58%	0.068%
93	12.877	3657	3666	3685	rBV3	18380	32048	2.73%	0.317%
94	12.958	3687	3691	3694	rBV3	390	341	0.03%	0.003%
95	13.106	3733	3737	3739	rBV3	453	373	0.03%	0.004%
96	13.221	3770	3773	3777	rBV	391	339	0.03%	0.003%
97	13.492	3849	3857	3876	rBV2	19695	35690	3.05%	0.354%
98	13.733	3923	3932	3948	rBV2	28869	55178	4.71%	0.547%
99	13.977	3999	4008	4023	rBV2	22132	41386	3.53%	0.410%
100	14.649	4214	4217	4221	rBV2	659	500	0.04%	0.005%


Sum of corrected areas: 10095006

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU073119\
Data File : VU033497.D
Acq On : 30 Jul 2019 16:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

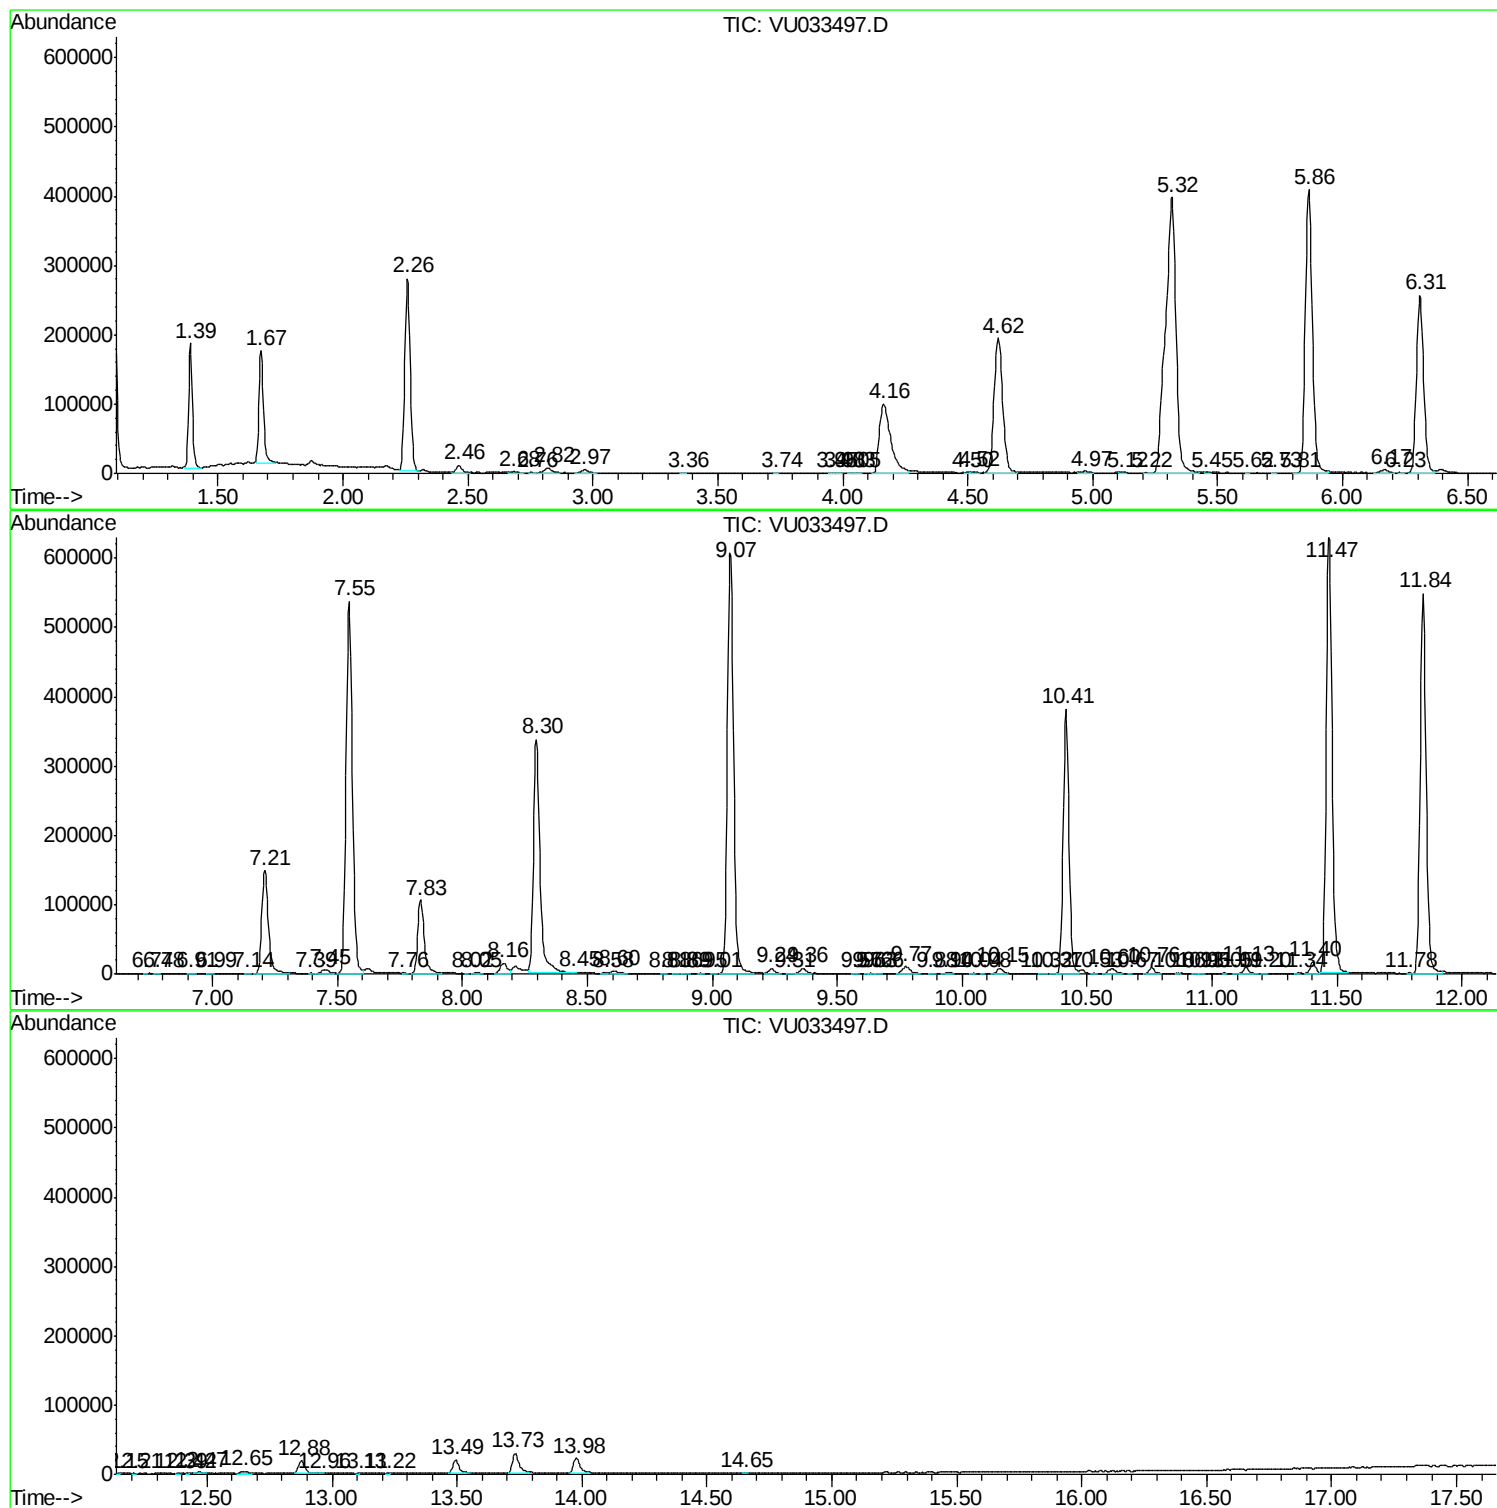

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033497.D
Acq On : 30 Jul 2019 16:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033497.D
Acq On : 30 Jul 2019 16:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc