

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033517.D
 Acq On : 31 Jul 2019 11:53
 Operator : JC/SP
 Sample : K4103-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	87	93	105	rVB	164991	175612	15.33%	1.957%
2	1.669	174	180	195	rVB	138798	175781	15.35%	1.958%
3	2.257	353	363	376	rVB	265167	405281	35.39%	4.515%
4	2.421	411	414	418	rBV2	500	382	0.03%	0.004%
5	2.556	448	456	459	rBV3	350	545	0.05%	0.006%
6	2.675	490	493	495	rBV	592	448	0.04%	0.005%
7	2.814	534	536	538	rVB	179	48	0.00%	0.001%
8	2.904	562	564	566	rBV2	216	130	0.01%	0.001%
9	3.016	596	599	603	rBV2	252	198	0.02%	0.002%
10	3.064	612	614	618	rVB2	269	116	0.01%	0.001%
11	3.106	622	627	632	rBV2	228	266	0.02%	0.003%
12	3.135	632	636	641	rVB2	305	240	0.02%	0.003%
13	3.283	677	682	689	rBV	234	270	0.02%	0.003%
14	3.318	689	693	694	rBV	158	101	0.01%	0.001%
15	3.344	699	701	704	rBV	257	113	0.01%	0.001%
16	3.363	704	707	713	rVB3	273	263	0.02%	0.003%
17	3.399	716	718	720	rVB3	159	64	0.01%	0.001%
18	3.424	722	726	729	rBV	135	131	0.01%	0.001%
19	3.463	735	738	741	rBV2	111	94	0.01%	0.001%
20	3.515	752	754	756	rBV	81	40	0.00%	0.000%
21	3.553	762	766	773	rVB	247	256	0.02%	0.003%
22	3.598	777	780	783	rBV3	227	183	0.02%	0.002%
23	3.614	783	785	786	rVV	172	48	0.00%	0.001%
24	3.624	786	788	790	rVB2	216	75	0.01%	0.001%
25	3.724	816	819	822	rVB2	256	145	0.01%	0.002%
26	3.785	836	838	842	rVB	234	125	0.01%	0.001%
27	3.810	842	846	847	rBV	123	82	0.01%	0.001%
28	3.836	852	854	855	rBV	116	34	0.00%	0.000%
29	3.936	879	885	889	rBB2	167	154	0.01%	0.002%
30	3.958	889	892	899	rVB2	138	134	0.01%	0.001%
31	3.994	899	903	905	rBV	247	183	0.02%	0.002%
32	4.045	917	919	920	rBV	166	48	0.00%	0.001%
33	4.055	920	922	925	rVB	171	86	0.01%	0.001%
34	4.151	940	952	982	rBV	97610	266610	23.28%	2.970%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033517.D
 Acq On : 31 Jul 2019 11:53
 Operator : JC/SP
 Sample : K4103-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

35	4.527	1064	1069	1072	rBV2	225	288	0.03%	0.003%
36	4.621	1080	1098	1130	rBV	192207	459564	40.13%	5.120%
37	4.932	1192	1195	1197	rBV	135	69	0.01%	0.001%
38	5.016	1220	1221	1222	rBV	155	52	0.00%	0.001%
39	5.080	1238	1241	1244	rVB2	87	54	0.00%	0.001%
40	5.106	1247	1249	1256	rVB2	309	236	0.02%	0.003%
41	5.138	1256	1259	1262	rBV2	71	63	0.01%	0.001%
42	5.158	1262	1265	1268	rVB2	159	83	0.01%	0.001%
43	5.174	1268	1270	1272	rBV2	67	35	0.00%	0.000%
44	5.228	1285	1287	1289	rBV	70	35	0.00%	0.000%
45	5.318	1291	1315	1347	rVV2	387029	1145183	100.00%	12.759%
46	5.627	1409	1411	1414	rBV2	108	68	0.01%	0.001%
47	5.694	1428	1432	1435	rBV3	215	193	0.02%	0.002%
48	5.714	1435	1438	1439	rVV2	275	135	0.01%	0.002%
49	5.727	1439	1442	1445	rVV3	290	242	0.02%	0.003%
50	5.752	1447	1450	1451	rBV2	224	109	0.01%	0.001%
51	5.794	1460	1463	1465	rBV3	260	177	0.02%	0.002%
52	5.865	1469	1485	1513	rBV	370083	719644	62.84%	8.018%
53	6.164	1572	1578	1579	rBV3	3584	3279	0.29%	0.037%
54	6.309	1608	1623	1646	rBV	259116	515786	45.04%	5.746%
55	6.524	1688	1690	1692	rBV	182	89	0.01%	0.001%
56	6.582	1705	1708	1709	rBV	154	74	0.01%	0.001%
57	6.620	1717	1720	1722	rBV	222	118	0.01%	0.001%
58	6.746	1756	1759	1763	rBV2	142	120	0.01%	0.001%
59	6.768	1763	1766	1773	rVB2	173	147	0.01%	0.002%
60	6.794	1773	1774	1777	rBV	119	51	0.00%	0.001%
61	6.813	1778	1780	1782	rBV2	205	89	0.01%	0.001%
62	6.829	1782	1785	1786	rBV	122	61	0.01%	0.001%
63	6.903	1805	1808	1811	rVB	197	121	0.01%	0.001%
64	6.942	1818	1820	1822	rVB2	220	77	0.01%	0.001%
65	6.955	1822	1824	1825	rBV2	154	65	0.01%	0.001%
66	6.987	1831	1834	1837	rBV2	202	114	0.01%	0.001%
67	7.077	1860	1862	1865	rVB2	172	83	0.01%	0.001%
68	7.103	1865	1870	1872	rBV2	143	107	0.01%	0.001%
69	7.119	1872	1875	1877	rBV	163	102	0.01%	0.001%
70	7.209	1891	1903	1927	rBV	138603	255947	22.35%	2.852%
71	7.476	1984	1986	1988	rVB2	138	53	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033517.D
 Acq On : 31 Jul 2019 11:53
 Operator : JC/SP
 Sample : K4103-04 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

72	7.547	1995	2008	2042	rBV	520046	908712	79.35%	10.124%
73	7.833	2086	2097	2127	rBV	99896	177354	15.49%	1.976%
74	8.042	2160	2162	2163	rBV	154	47	0.00%	0.001%
75	8.096	2177	2179	2180	rBV	143	38	0.00%	0.000%
76	8.209	2211	2214	2216	rBV3	949	622	0.05%	0.007%
77	8.296	2230	2241	2268	rBV	322431	572769	50.02%	6.381%
78	8.730	2374	2376	2379	rBV	224	115	0.01%	0.001%
79	8.817	2399	2403	2407	rVB2	469	406	0.04%	0.005%
80	8.836	2407	2409	2412	rVB	209	109	0.01%	0.001%
81	8.858	2412	2416	2419	rBV2	233	192	0.02%	0.002%
82	8.932	2435	2439	2441	rBV	270	186	0.02%	0.002%
83	8.948	2441	2444	2445	rBV	182	81	0.01%	0.001%
84	9.071	2469	2482	2505	rBV	537874	906802	79.18%	10.103%
85	9.267	2541	2543	2545	rBV	387	224	0.02%	0.002%
86	9.357	2568	2571	2572	rBV	389	187	0.02%	0.002%
87	9.553	2630	2632	2635	rVB	213	92	0.01%	0.001%
88	9.656	2662	2664	2670	rVB	226	175	0.02%	0.002%
89	9.717	2682	2683	2685	rBV	242	79	0.01%	0.001%
90	9.868	2727	2730	2732	rBV2	213	130	0.01%	0.001%
91	10.112	2803	2806	2809	rBV2	231	201	0.02%	0.002%
92	10.189	2825	2830	2833	rBV2	452	405	0.04%	0.005%
93	10.234	2841	2844	2846	rBV2	129	60	0.01%	0.001%
94	10.415	2888	2900	2924	rBV	380609	605751	52.90%	6.749%
95	11.013	3084	3086	3087	rBV	244	117	0.01%	0.001%
96	11.408	3203	3209	3215	rBV4	663	993	0.09%	0.011%
97	11.469	3216	3228	3248	rBV	525396	835860	72.99%	9.312%
98	11.842	3332	3344	3368	rBV	511438	832472	72.69%	9.275%
99	12.218	3459	3461	3462	rBV	618	219	0.02%	0.002%
100	12.550	3562	3564	3569	rBV4	381	345	0.03%	0.004%


Sum of corrected areas: 8975742

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU073119\
Data File : VU033517.D
Acq On : 31 Jul 2019 11:53
Operator : JC/SP
Sample : K4103-04 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

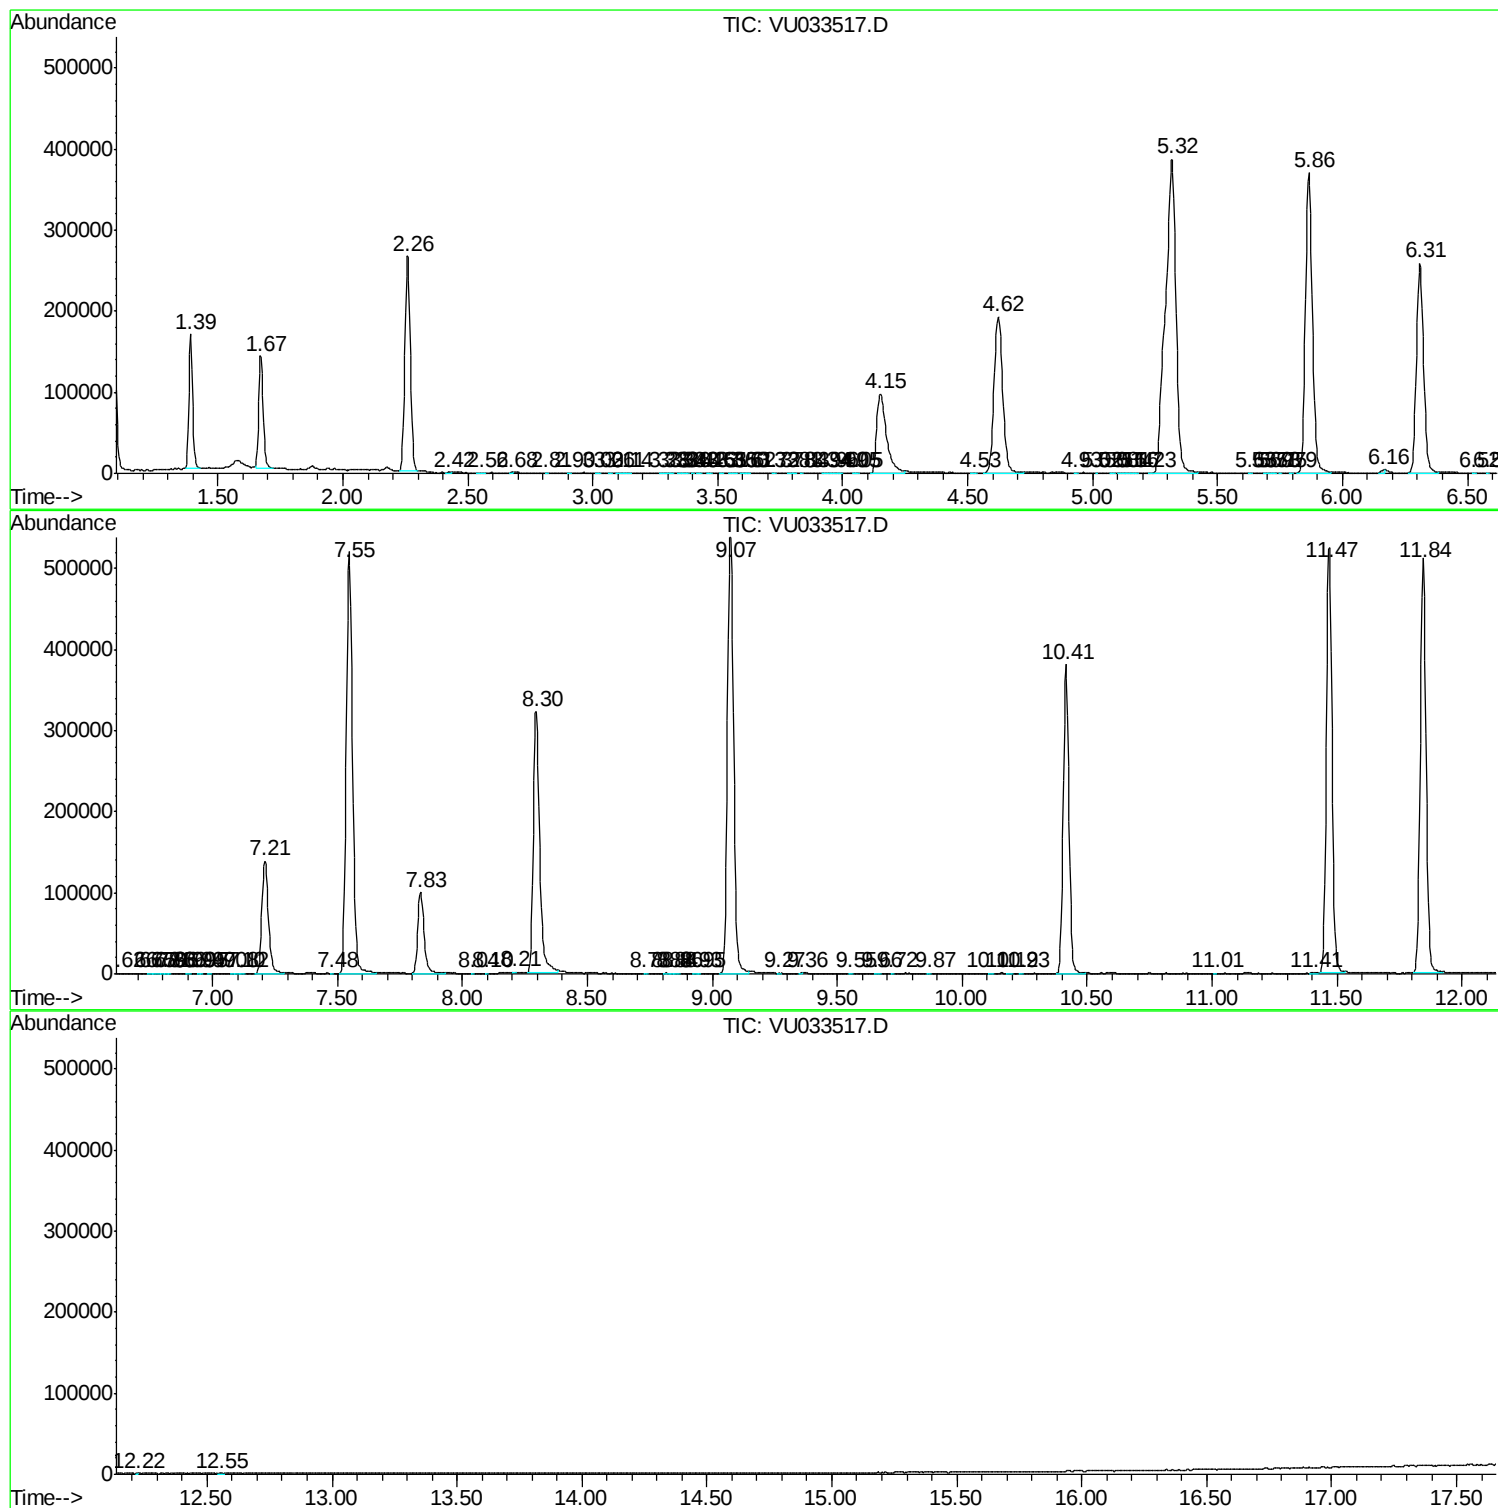

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033517.D
Acq On : 31 Jul 2019 11:53
Operator : JC/SP
Sample : K4103-04 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033517.D
Acq On : 31 Jul 2019 11:53
Operator : JC/SP
Sample : K4103-04 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc