

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033533.D
 Acq On : 31 Jul 2019 18:23
 Operator : JC/SP
 Sample : K4103-10DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9E6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	86	93	108	rBV	153969	161827	14.83%	1.788%
2	1.550	137	143	151	rVB2	19850	24831	2.28%	0.274%
3	1.669	172	180	196	rBV	128180	162183	14.87%	1.792%
4	2.257	353	363	376	rVB	268311	403253	36.97%	4.456%
5	2.354	391	393	397	rVV3	330	185	0.02%	0.002%
6	2.373	397	399	402	rVB2	383	181	0.02%	0.002%
7	2.415	407	412	413	rBV	293	221	0.02%	0.002%
8	2.460	423	426	431	rVB4	541	368	0.03%	0.004%
9	2.688	489	497	509	rVB4	1804	2956	0.27%	0.033%
10	2.820	526	538	552	rVV	5828	11240	1.03%	0.124%
11	2.964	577	583	590	rBV3	665	791	0.07%	0.009%
12	3.328	694	696	700	rVB	313	195	0.02%	0.002%
13	3.363	704	707	712	rVB2	439	297	0.03%	0.003%
14	3.505	747	751	756	rVB2	179	198	0.02%	0.002%
15	3.653	793	797	801	rBV2	222	163	0.01%	0.002%
16	3.730	814	821	824	rBV	198	234	0.02%	0.003%
17	3.794	837	841	846	rVB	196	217	0.02%	0.002%
18	4.151	938	952	959	rBV	105922	248670	22.80%	2.748%
19	4.399	1027	1029	1035	rBV2	417	389	0.04%	0.004%
20	4.427	1035	1038	1044	rVB3	559	540	0.05%	0.006%
21	4.543	1072	1074	1079	rVB3	492	343	0.03%	0.004%
22	4.624	1079	1099	1127	rBV	182399	441884	40.51%	4.883%
23	4.781	1146	1148	1150	rBV2	317	157	0.01%	0.002%
24	4.852	1166	1170	1173	rBV3	466	399	0.04%	0.004%
25	4.903	1183	1186	1189	rVB2	311	228	0.02%	0.003%
26	4.929	1189	1194	1196	rBV	210	185	0.02%	0.002%
27	4.961	1201	1204	1205	rBV	353	183	0.02%	0.002%
28	4.974	1206	1208	1213	rVB2	429	296	0.03%	0.003%
29	5.051	1227	1232	1235	rVB2	219	153	0.01%	0.002%
30	5.132	1254	1257	1261	rBV2	308	191	0.02%	0.002%
31	5.157	1261	1265	1270	rVB2	208	221	0.02%	0.002%
32	5.315	1290	1314	1342	rBV2	368851	1090881	100.00%	12.055%
33	5.534	1380	1382	1388	rVB2	390	228	0.02%	0.003%
34	5.575	1392	1395	1399	rBV2	239	212	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U073119\
 Data File : VU033533.D
 Acq On : 31 Jul 2019 18:23
 Operator : JC/SP
 Sample : K4103-10DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9E6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

35	5.691	1428	1431	1434	rBV2	286	195	0.02%	0.002%
36	5.816	1465	1470	1472	rBV3	265	185	0.02%	0.002%
37	5.865	1472	1485	1512	rBV	349231	682034	62.52%	7.537%
38	6.167	1565	1579	1596	rBV	191807	366682	33.61%	4.052%
39	6.308	1609	1623	1649	rBV	247637	495202	45.39%	5.472%
40	6.434	1659	1662	1664	rBV2	474	345	0.03%	0.004%
41	6.447	1664	1666	1669	rVB2	663	356	0.03%	0.004%
42	6.852	1785	1792	1799	rBV5	768	1105	0.10%	0.012%
43	6.932	1814	1817	1822	rBV2	314	258	0.02%	0.003%
44	7.209	1891	1903	1928	rBV2	131921	239214	21.93%	2.643%
45	7.308	1931	1934	1936	rVV	347	166	0.02%	0.002%
46	7.386	1951	1958	1959	rBV2	334	322	0.03%	0.004%
47	7.395	1959	1961	1964	rVB	375	200	0.02%	0.002%
48	7.447	1973	1977	1979	rBV2	618	532	0.05%	0.006%
49	7.482	1985	1988	1991	rVB2	331	191	0.02%	0.002%
50	7.546	1992	2008	2030	rBV	492320	851195	78.03%	9.406%
51	7.832	2086	2097	2125	rBV	94842	168601	15.46%	1.863%
52	7.977	2140	2142	2146	rBV3	207	170	0.02%	0.002%
53	8.054	2161	2166	2169	rBV3	202	221	0.02%	0.002%
54	8.122	2184	2187	2190	rBV2	244	157	0.01%	0.002%
55	8.164	2190	2200	2208	rBV2	1725	2794	0.26%	0.031%
56	8.295	2229	2241	2274	rBV	321856	573126	52.54%	6.333%
57	8.582	2326	2330	2335	rBV4	320	314	0.03%	0.003%
58	8.784	2390	2393	2398	rVB	373	173	0.02%	0.002%
59	8.810	2398	2401	2404	rVB2	247	156	0.01%	0.002%
60	8.887	2421	2425	2430	rVB3	405	350	0.03%	0.004%
61	8.935	2430	2440	2443	rBV2	246	331	0.03%	0.004%
62	8.971	2447	2451	2454	rBV3	281	221	0.02%	0.002%
63	9.070	2470	2482	2510	rBV	526797	876760	80.37%	9.689%
64	9.231	2530	2532	2537	rVB2	373	314	0.03%	0.003%
65	9.646	2658	2661	2663	rBV2	262	154	0.01%	0.002%
66	9.765	2695	2698	2704	rBV3	267	294	0.03%	0.003%
67	9.810	2710	2712	2717	rBV2	236	200	0.02%	0.002%
68	9.836	2717	2720	2722	rVV2	297	164	0.02%	0.002%
69	9.858	2722	2727	2732	rVV2	269	314	0.03%	0.003%
70	9.884	2732	2735	2739	rVV	238	161	0.01%	0.002%
71	9.913	2741	2744	2748	rVB	494	336	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
 Data File : VU033533.D
 Acq On : 31 Jul 2019 18:23
 Operator : JC/SP
 Sample : K4103-10DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9E6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

72	9.932	2748	2750	2753	rBV	242	169	0.02%	0.002%
73	10.019	2774	2777	2783	rBV2	153	167	0.02%	0.002%
74	10.061	2788	2790	2793	rVB2	342	172	0.02%	0.002%
75	10.331	2872	2874	2880	rVB2	257	166	0.02%	0.002%
76	10.414	2887	2900	2928	rBV	378275	603171	55.29%	6.665%
77	10.598	2952	2957	2959	rBV2	329	310	0.03%	0.003%
78	10.675	2974	2981	2982	rBV2	308	319	0.03%	0.004%
79	10.768	3005	3010	3013	rBV	189	182	0.02%	0.002%
80	10.813	3022	3024	3027	rBV	357	223	0.02%	0.002%
81	10.871	3040	3042	3045	rVV2	314	176	0.02%	0.002%
82	10.948	3063	3066	3069	rBV	323	174	0.02%	0.002%
83	11.000	3079	3082	3085	rVB2	295	178	0.02%	0.002%
84	11.125	3119	3121	3123	rBV2	361	164	0.02%	0.002%
85	11.154	3128	3130	3134	rBV2	377	282	0.03%	0.003%
86	11.250	3157	3160	3164	rBV	382	246	0.02%	0.003%
87	11.401	3205	3207	3210	rVB	302	167	0.02%	0.002%
88	11.469	3215	3228	3247	rBV	499820	810040	74.26%	8.951%
89	11.739	3309	3312	3317	rBV3	484	490	0.04%	0.005%
90	11.768	3318	3321	3329	rVB	475	420	0.04%	0.005%
91	11.845	3332	3345	3365	rBV	504437	811313	74.37%	8.965%
92	12.038	3402	3405	3407	rBV2	625	422	0.04%	0.005%
93	12.115	3427	3429	3433	rBV	285	222	0.02%	0.002%
94	12.157	3440	3442	3448	rVB2	251	197	0.02%	0.002%
95	12.331	3492	3496	3502	rBV3	318	512	0.05%	0.006%
96	12.533	3554	3559	3560	rBV2	390	265	0.02%	0.003%
97	12.758	3626	3629	3632	rBV3	308	241	0.02%	0.003%
98	12.819	3646	3648	3650	rBV2	247	154	0.01%	0.002%
99	13.028	3708	3713	3719	rBV4	517	720	0.07%	0.008%
100	13.260	3783	3785	3788	rBV2	330	184	0.02%	0.002%


Sum of corrected areas: 9049439

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU073119\
Data File : VU033533.D
Acq On : 31 Jul 2019 18:23
Operator : JC/SP
Sample : K4103-10DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9E6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

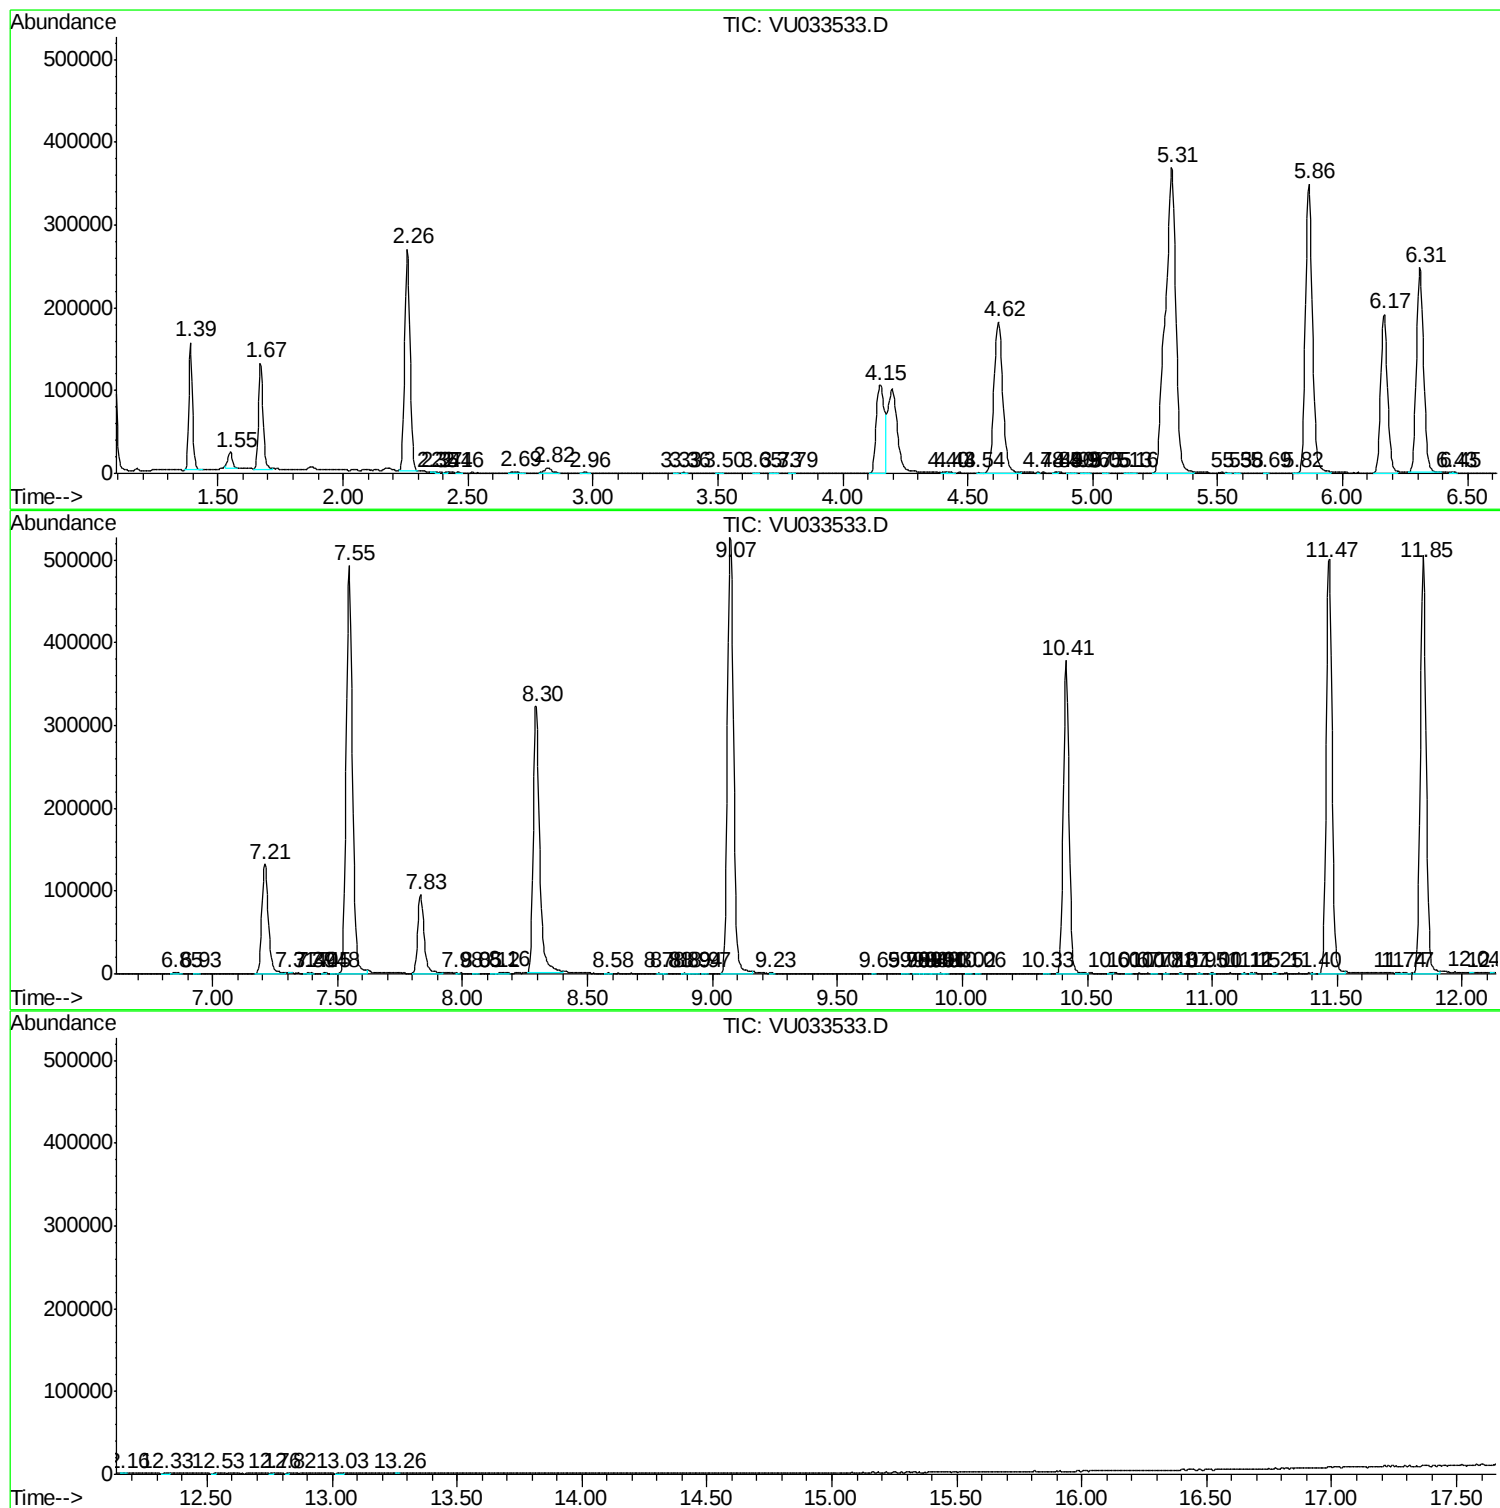

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033533.D
Acq On : 31 Jul 2019 18:23
Operator : JC/SP
Sample : K4103-10DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9E6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU073119\
Data File : VU033533.D
Acq On : 31 Jul 2019 18:23
Operator : JC/SP
Sample : K4103-10DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9E6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc