


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU073119\
Data File : VU033491.D
Acq On : 30 Jul 2019 14:29
Operator : JC/SP
Sample : BFB42
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Title : VOC Analysis
Last Update : Thu Aug 01 14:08:00 2019

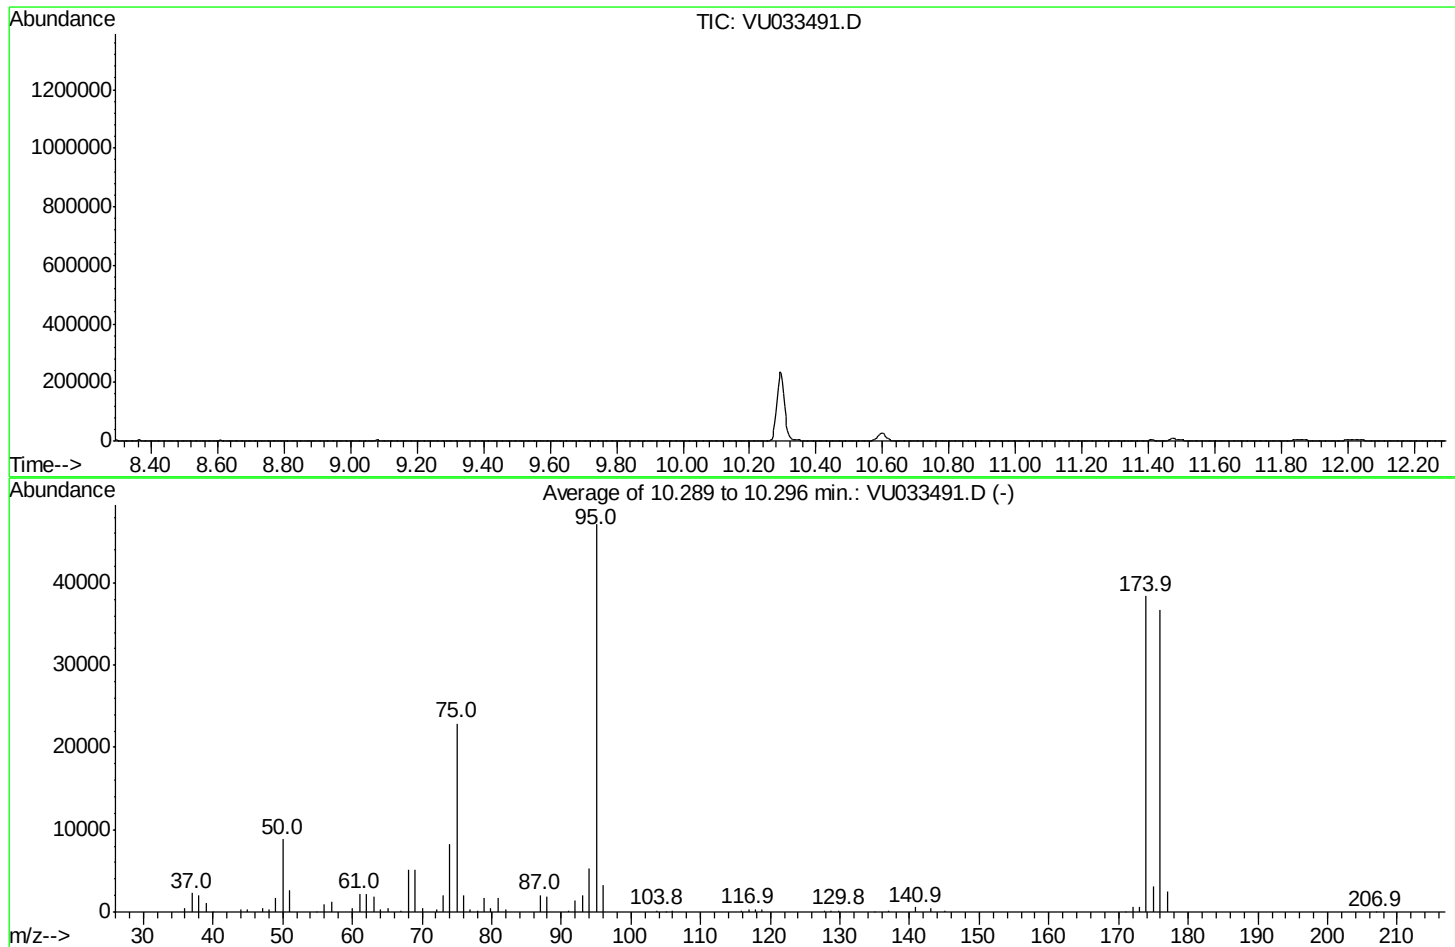

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	8820	PASS
75	95	30	80	48.5	22874	PASS
95	95	100	100	100.0	47125	PASS
96	95	5	9	7.0	3276	PASS
173	174	0.00	2	1.7	643	PASS
174	95	50	120	81.5	38421	PASS
175	174	5	9	8.0	3092	PASS
176	174	95	101	95.6	36725	PASS
177	176	5	9	6.7	2477	PASS

Scan 2850 (10.254 min): VU033491.D
BFB42

m/z	Abundance
39.90	234.0
44.00	360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	420.0
37.00	2270.0
38.00	2001.0
39.00	1023.0
39.90	296.0
44.00	616.0
44.90	401.0
47.10	383.0
48.00	232.0
49.00	1619.0
50.00	8710.0
51.00	2632.0
56.00	882.0
57.00	1224.0
60.00	349.0
61.00	2111.0
62.10	1852.0
63.10	1809.0
64.00	272.0
65.00	350.0
66.90	145.0
68.00	4820.0
69.00	5072.0
70.00	391.0
72.10	261.0
73.00	1943.0
74.00	7908.0
75.00	22480.0
76.00	2158.0
76.90	419.0
78.10	239.0
78.90	1625.0
79.90	402.0
80.90	1767.0
82.00	398.0
86.90	1978.0
87.90	1942.0
91.10	176.0
92.00	1309.0
93.00	1877.0
94.00	5040.0
95.00	46000.0
96.00	3132.0
103.80	187.0
105.90	187.0
115.90	183.0
116.90	283.0
117.80	244.0
118.80	271.0
127.80	168.0
128.80	105.0
129.80	219.0
137.00	102.0
140.90	497.0
142.90	516.0
145.00	251.0
172.10	537.0
173.00	638.0
173.90	35616.0
175.00	2846.0
176.00	34648.0
177.00	2385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	461.0
37.00	2413.0
38.00	2051.0
39.00	1100.0
39.90	259.0
43.90	639.0
44.90	391.0
47.10	417.0
48.00	258.0
49.00	1791.0
50.00	9167.0
51.00	2703.0
56.00	955.0
57.00	1281.0
59.90	425.0
61.00	2329.0
62.10	2211.0
63.10	1899.0
64.00	274.0
65.10	415.0
66.90	153.0
68.00	5256.0
69.00	5231.0
70.00	452.0
72.10	273.0
73.00	2113.0
74.00	8555.0
75.00	23608.0
76.10	2189.0
76.90	354.0
78.10	243.0
78.90	1728.0
79.90	452.0
80.90	1821.0
82.00	409.0
87.00	2089.0
88.00	1951.0
91.00	201.0
92.00	1452.0
93.00	2099.0
94.00	5420.0
95.00	48880.0
96.00	3421.0
103.80	210.0
105.90	159.0
115.90	181.0
116.90	385.0
117.90	250.0
118.80	290.0
127.90	197.0
128.70	105.0
129.90	210.0
134.90	105.0
136.90	126.0
140.90	591.0
142.90	564.0
145.00	249.0
170.90	125.0
172.00	622.0
173.00	655.0
173.90	39576.0
175.00	3167.0
176.00	37792.0
177.00	2542.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	411.0
37.00	2231.0
38.00	1939.0
39.00	1046.0
39.90	246.0
43.90	626.0
44.90	326.0
47.20	402.0
48.00	261.0
49.00	1759.0
50.00	8584.0
51.00	2567.0
54.90	110.0
56.00	896.0
57.00	1278.0
59.90	450.0
61.00	2222.0
62.00	2383.0
63.10	1820.0
64.00	261.0
65.10	476.0
66.90	123.0
68.00	5163.0
69.00	4958.0
70.00	383.0
72.10	228.0
73.00	1978.0
74.00	8284.0
75.00	22536.0
76.10	1964.0
76.90	274.0
78.00	227.0
78.90	1664.0
79.90	480.0
80.90	1641.0
82.00	343.0
87.00	2038.0
88.00	1794.0
91.00	199.0
92.00	1374.0
93.00	2172.0
94.00	5320.0
95.00	46496.0
96.00	3275.0
103.80	208.0
105.00	108.0
106.00	146.0
115.90	150.0
116.90	405.0
117.90	245.0
118.80	274.0
127.90	201.0
128.70	105.0
129.90	154.0
136.90	111.0
140.90	668.0
143.00	560.0
145.00	205.0
170.90	126.0
171.90	710.0
173.00	636.0
174.00	40072.0
175.00	3264.0
176.00	37736.0
177.00	2504.0
206.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42