


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU073120\
 Data File : VU039728.D
 Acq On : 31 Jul 2020 10:34
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072920DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jul 31 07:12:27 2020

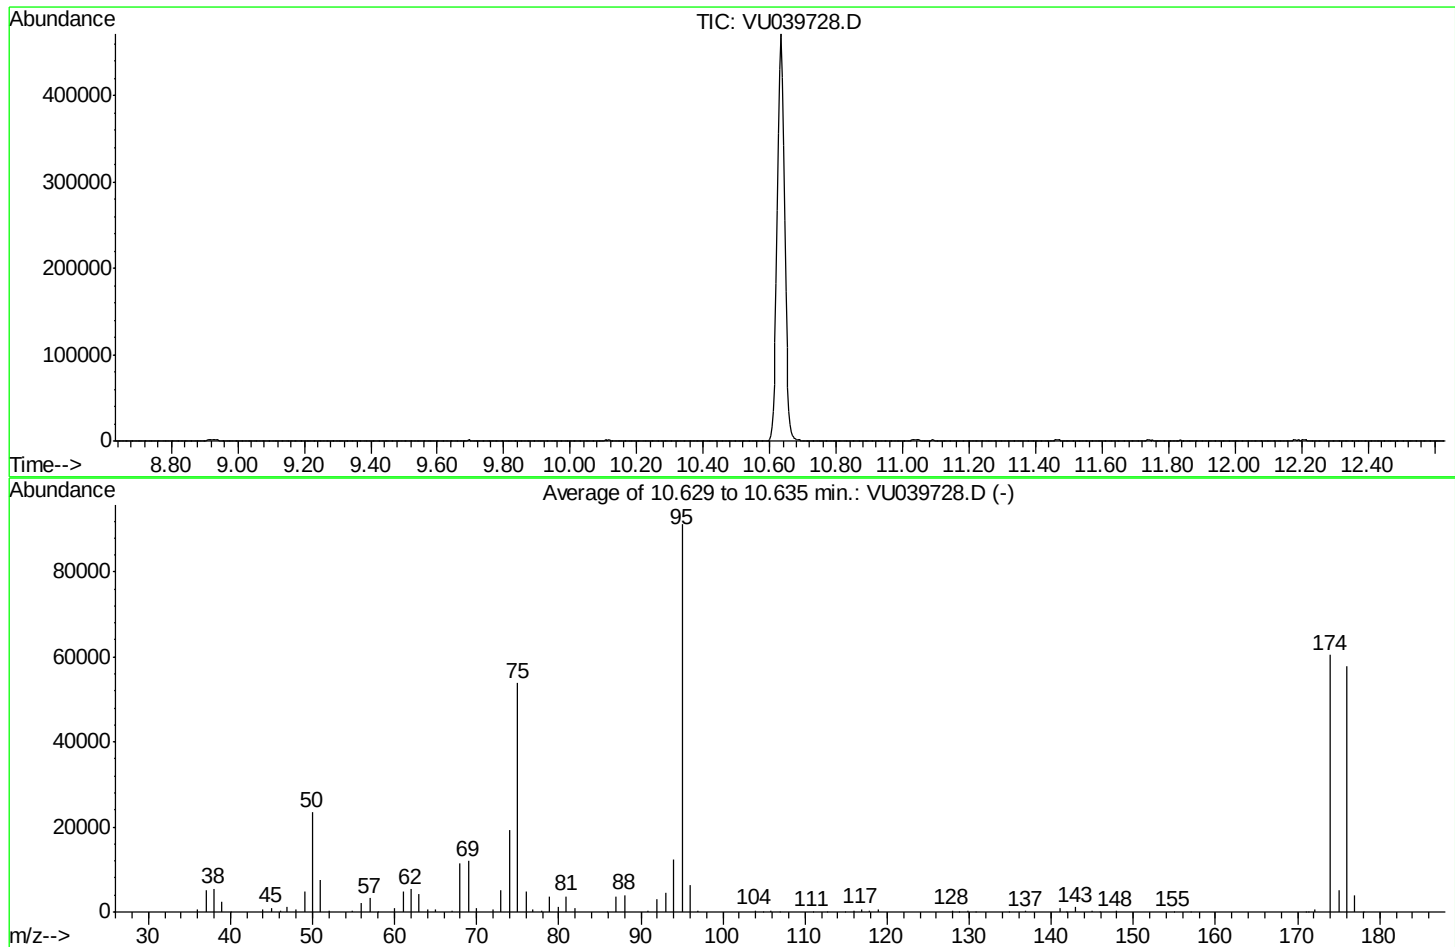

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.7	23421	PASS
75	95	30	60	59.1	53874	PASS
95	95	100	100	100.0	91197	PASS
96	95	5	9	6.8	6184	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.3	60469	PASS
175	174	5	9	8.4	5088	PASS
176	174	95	101	95.7	57896	PASS
177	176	5	9	7.0	4058	PASS