

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073124\
 Data File : VU060275.D
 Acq On : 31 Jul 2024 11:37
 Operator : MD/SY
 Sample : VU0731MBL01
 Misc : 5.00g/5.0mL//100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Aug 01 00:20:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 01 00:19:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	234001	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	235113	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	89178	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	88249	58.737	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 117.480%			
7) Chloroethane-d5	1.901	69	67754	53.613	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 107.220%			
11) 1,1-Dichloroethene-d2	2.557	63	102209	38.292	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 76.580%			
21) 2-Butanone-d5	4.611	46	111344	106.637	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 106.640%			
24) Chloroform-d	5.052	84	135834	46.686	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.380%			
26) 1,2-Dichloroethane-d4	5.692	65	82763	47.841	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 95.680%			
32) Benzene-d6	5.718	84	285284	47.385	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 94.780%			
36) 1,2-Dichloropropane-d6	6.682	67	96556	51.818	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 103.640%			
41) Toluene-d8	7.891	98	233045	40.704	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 81.400%			
43) trans-1,3-Dichloroprop...	8.174	79	38092	43.687	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 87.380%			
47) 2-Hexanone-d5	8.624	63	63751	81.181	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 81.180%			
56) 1,1,2,2-Tetrachloroeth...	10.749	84	135048	47.219	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 94.440%			
66) 1,2-Dichlorobenzene-d4	12.187	152	78491	47.897	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 95.800%			
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	9665	5.531	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073124\
Data File : VU060275.D
Acq On : 31 Jul 2024 11:37
Operator : MD/SY
Sample : VU0731MBL01
Misc : 5.00g/5.0mL//100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Aug 01 00:20:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 01 00:19:02 2024
Response via : Initial Calibration

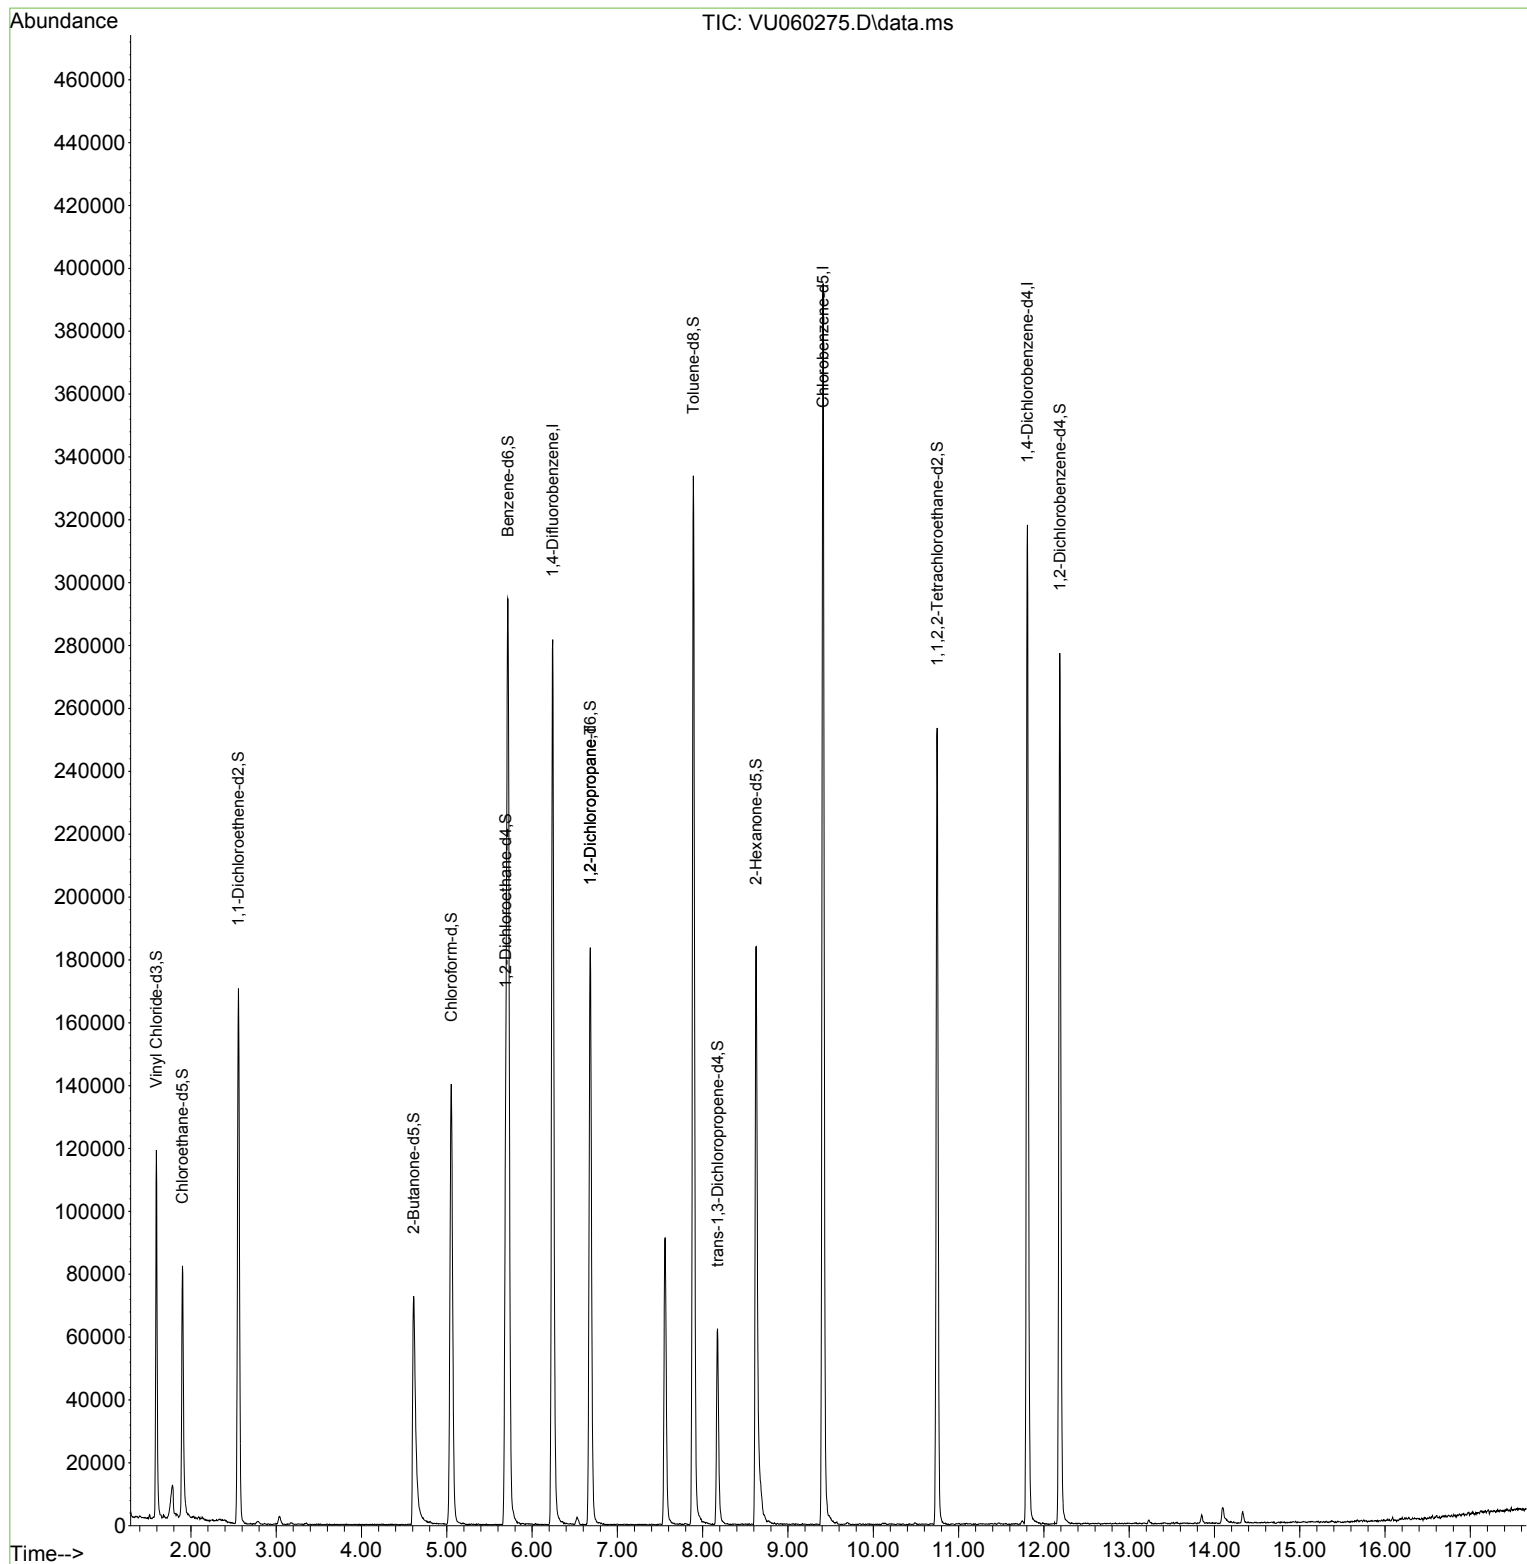

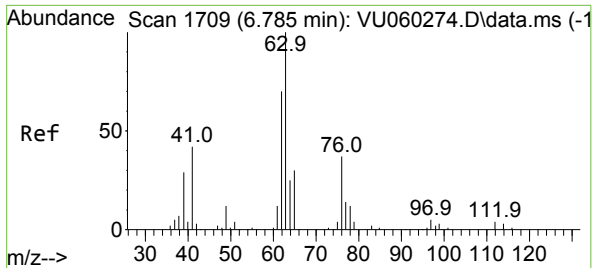

#37
1,2-Dichloropropane
Concen: 5.531 ug/L
RT: 6.682 min Scan# 1
Delta R.T. -0.103 min
Lab File: VU060275.D
Acq: 31 Jul 2024 11:37

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 9665
Ion Ratio Lower Upper
63 100
112 0.0 3.0 4.6#

