


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU073124\
Data File : VU060273.D
Acq On : 31 Jul 2024 08:50
Operator : MD/SY
Sample : BFB075
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB075

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Thu Aug 01 00:19:02 2024

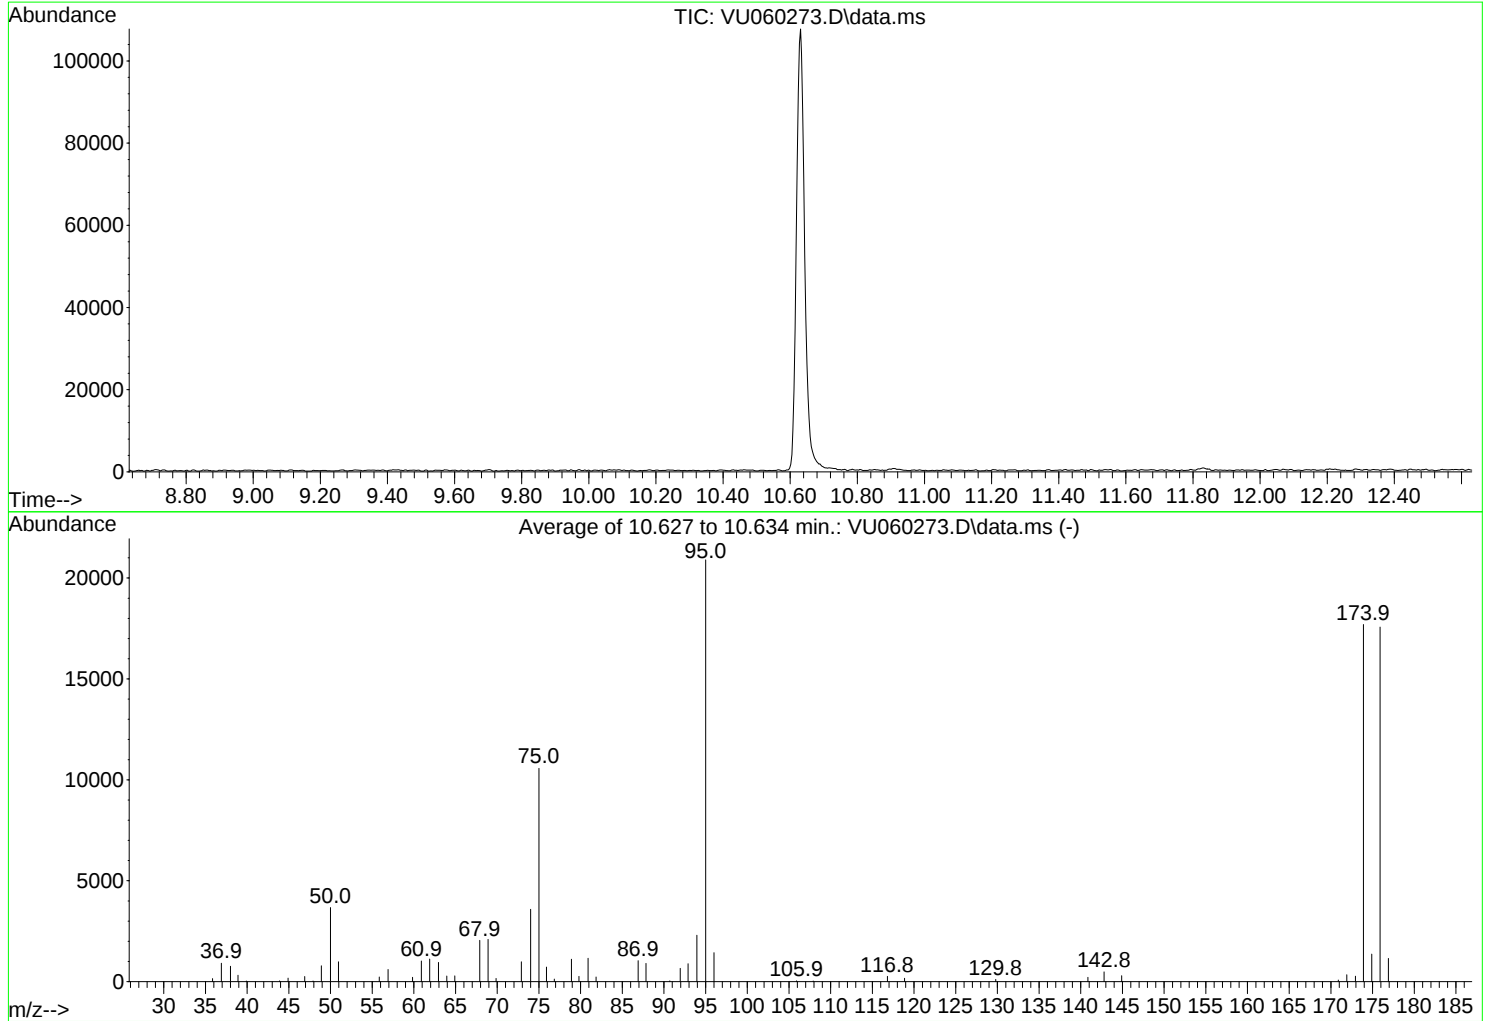

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	3673	PASS
75	95	30	80	50.6	10570	PASS
95	95	100	100	100.0	20901	PASS
96	95	5	9	6.9	1435	PASS
173	174	0.00	2	1.5	270	PASS
174	95	50	120	84.7	17693	PASS
175	174	5	9	7.7	1362	PASS
176	174	95	101	99.3	17571	PASS
177	176	5	9	6.6	1151	PASS

m/z	Abundance
39.90	128.0
43.90	351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.90	206.0
36.90	925.0
38.00	832.0
38.90	281.0
40.10	158.0
43.90	356.0
44.90	217.0
46.90	276.0
47.90	101.0
48.90	783.0
50.00	3663.0
50.90	1101.0
55.80	213.0
56.90	653.0
59.90	207.0
60.90	1099.0
61.90	1051.0
63.00	946.0
63.90	287.0
64.90	240.0
67.90	2094.0
68.90	1943.0
69.80	209.0
72.90	923.0
74.00	3512.0
75.00	10691.0
75.90	808.0
76.80	123.0
78.90	1066.0
79.80	224.0
80.90	1150.0
81.80	261.0
86.90	1064.0
87.80	868.0
91.90	580.0
92.90	858.0
94.00	2398.0
95.00	20992.0
96.00	1431.0
105.90	121.0
116.80	204.0
118.90	143.0
129.80	101.0
141.00	212.0
142.80	478.0
144.90	279.0
170.90	123.0
171.90	311.0
173.00	256.0
173.90	17232.0
174.90	1433.0
175.90	17352.0
176.90	1189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.90	150.0
36.90	985.0
38.00	782.0
38.90	319.0
39.90	157.0
43.90	409.0
44.90	176.0
46.90	283.0
48.90	823.0
50.00	3823.0
51.00	988.0
55.90	237.0
56.90	644.0
59.80	212.0
60.90	1071.0
61.90	1171.0
62.90	996.0
64.00	277.0
64.90	310.0
67.90	2123.0
68.90	2190.0
69.90	163.0
72.90	1026.0
74.00	3693.0
75.00	10811.0
75.90	718.0
76.90	117.0
78.90	1157.0
79.80	283.0
80.90	1246.0
81.80	237.0
86.90	1085.0
87.90	932.0
90.70	110.0
92.00	675.0
92.90	914.0
94.00	2389.0
95.00	21344.0
96.00	1479.0
116.80	280.0
118.80	165.0
129.80	118.0
140.80	223.0
142.80	500.0
144.90	296.0
170.90	112.0
171.90	353.0
172.90	273.0
173.90	18240.0
174.90	1397.0
175.90	18096.0
176.90	1177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	100.0
36.90	832.0
38.00	662.0
38.90	349.0
39.80	160.0
43.90	407.0
44.90	126.0
46.90	207.0
48.90	739.0
50.00	3532.0
51.00	855.0
55.90	235.0
56.90	519.0
59.90	221.0
60.90	894.0
61.90	1124.0
62.90	907.0
64.00	257.0
64.90	313.0
67.90	1915.0
68.90	2152.0
69.90	107.0
72.90	1007.0
74.00	3535.0
75.00	10208.0
75.90	632.0
76.90	135.0
78.90	1115.0
79.80	279.0
80.90	1069.0
81.90	201.0
86.90	969.0
87.90	924.0
92.00	729.0
92.90	898.0
93.90	2114.0
95.00	20368.0
96.00	1395.0
107.90	104.0
116.80	300.0
118.80	196.0
129.80	105.0
140.70	219.0
142.80	480.0
144.90	296.0
171.90	372.0
172.90	281.0
173.90	17608.0
174.90	1257.0
175.90	17264.0
176.90	1088.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075