


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080118\
Data File : VU025759.D
Acq On : 01 Aug 2018 07:28
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Title : SW846 8260
Last Update : Tue Jul 31 16:07:47 2018

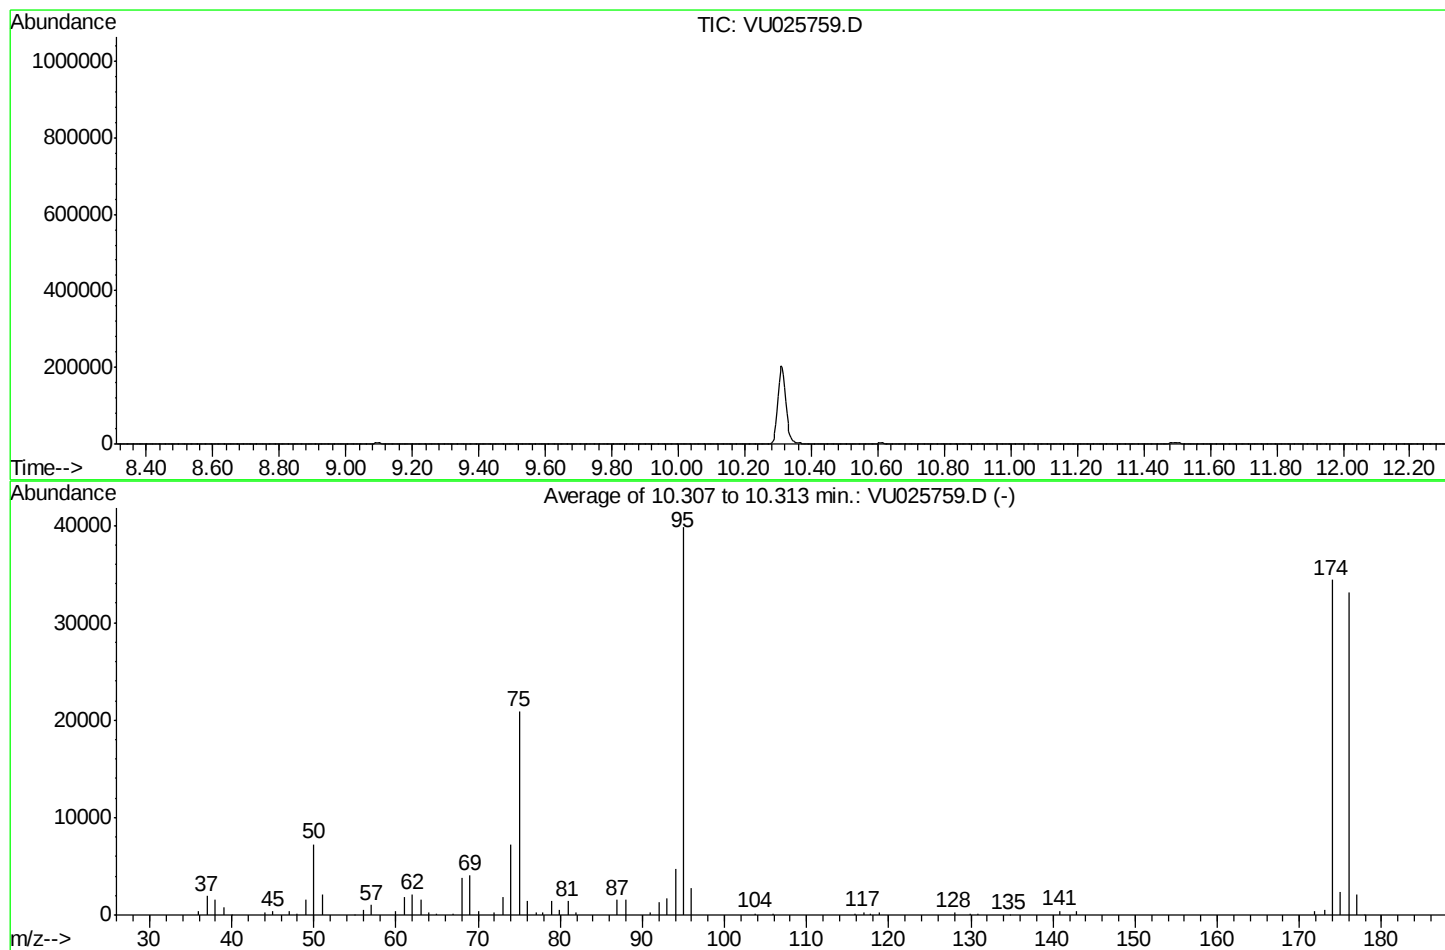

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	7242	PASS
75	95	30	60	52.4	20837	PASS
95	95	100	100	100.0	39786	PASS
96	95	5	9	6.8	2701	PASS
173	174	0.00	2	1.6	544	PASS
174	95	50	100	86.5	34413	PASS
175	174	5	9	7.0	2408	PASS
176	174	95	101	96.4	33160	PASS
177	176	5	9	6.3	2092	PASS