


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080119\
 Data File : VU033535.D
 Acq On : 01 Aug 2019 08:20
 Operator : JC/SP
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 02 12:05:52 2019

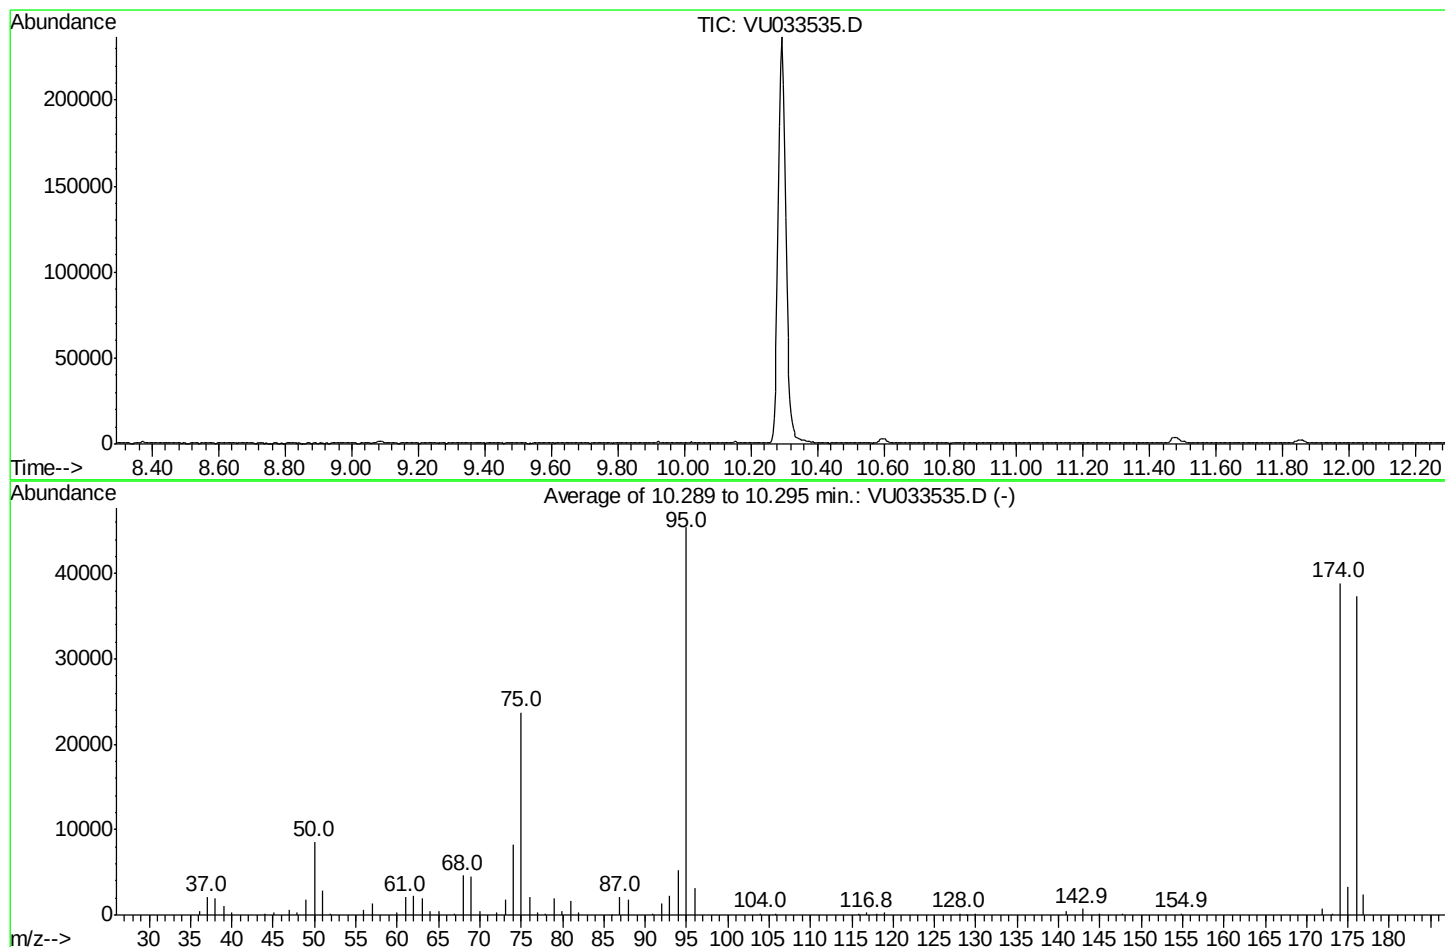

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8594	PASS
75	95	30	80	52.2	23714	PASS
95	95	100	100	100.0	45402	PASS
96	95	5	9	7.1	3210	PASS
173	174	0.00	2	0.6	229	PASS
174	95	50	120	85.7	38898	PASS
175	174	5	9	8.3	3235	PASS
176	174	95	101	95.9	37301	PASS
177	176	5	9	6.6	2457	PASS

Scan 2850 (10.254 min): VU033535.D
BFB44

m/z	Abundance
40.00	184.0
44.00	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.10	402.0
37.00	2142.0
38.00	1987.0
39.10	1073.0
40.00	360.0
43.90	546.0
45.10	418.0
46.90	460.0
47.90	279.0
49.00	1904.0
50.00	8600.0
51.00	3003.0
51.90	190.0
56.00	669.0
57.00	1375.0
60.00	352.0
61.00	2116.0
62.00	2244.0
63.00	1916.0
64.00	491.0
65.00	442.0
66.90	121.0
68.00	4297.0
69.00	4357.0
70.00	369.0
72.10	285.0
73.10	1693.0
74.00	7842.0
75.00	23000.0
76.00	1990.0
77.00	326.0
77.90	269.0
79.00	1820.0
79.90	368.0
81.00	1665.0
81.90	301.0
87.00	2115.0
88.00	1770.0
90.80	176.0
92.00	1261.0
93.00	2042.0
94.00	5014.0
95.00	44208.0
96.00	3036.0
103.90	185.0
105.90	174.0
115.80	130.0
116.80	232.0
118.00	161.0
118.90	260.0
128.00	176.0
128.80	116.0
129.90	112.0
141.00	412.0
142.90	724.0
145.00	210.0
147.80	103.0
154.80	206.0
171.90	642.0
173.10	688.0
174.00	36680.0
175.00	3042.0
176.00	34808.0
176.90	2354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	445.0
37.00	2212.0
38.00	2100.0
39.00	1117.0
40.00	473.0
43.90	497.0
45.00	391.0
47.00	596.0
47.90	253.0
49.00	1877.0
50.00	8894.0
51.00	2992.0
52.00	180.0
55.90	661.0
57.00	1529.0
60.00	385.0
61.00	2149.0
62.00	2371.0
63.10	2033.0
64.00	490.0
65.00	526.0
66.80	178.0
68.00	4809.0
69.00	4627.0
70.00	444.0
72.10	270.0
73.00	1881.0
74.00	8555.0
75.00	24504.0
76.00	2154.0
76.90	339.0
77.90	232.0
79.00	1990.0
79.90	450.0
80.90	1746.0
81.90	323.0
87.00	2198.0
88.00	1972.0
90.80	210.0
92.00	1403.0
93.00	2245.0
94.00	5328.0
95.00	46608.0
96.00	3341.0
103.90	223.0
105.80	201.0
115.80	182.0
116.80	304.0
117.90	204.0
119.00	273.0
128.00	198.0
128.80	110.0
129.90	171.0
141.00	435.0
142.90	715.0
145.00	212.0
147.80	110.0
154.90	200.0
171.90	743.0
174.00	40128.0
175.00	3341.0
176.00	38544.0
176.90	2507.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	407.0
37.00	2122.0
38.00	1908.0
39.00	1132.0
39.90	424.0
44.00	497.0
45.00	320.0
47.00	623.0
48.00	227.0
49.00	1705.0
50.00	8289.0
51.00	2728.0
52.00	164.0
55.90	649.0
57.00	1381.0
60.00	398.0
61.00	2076.0
62.00	2348.0
63.10	2138.0
64.00	421.0
65.00	515.0
66.90	183.0
68.00	4797.0
69.00	4498.0
70.00	470.0
72.10	241.0
73.00	1983.0
74.00	8346.0
75.00	23640.0
76.10	2104.0
76.90	290.0
77.90	163.0
78.90	1899.0
79.90	505.0
80.90	1756.0
81.90	334.0
85.90	117.0
86.90	2053.0
88.00	1863.0
90.90	246.0
92.00	1343.0
93.00	2262.0
94.00	5407.0
95.00	45392.0
96.00	3255.0
104.00	226.0
105.80	200.0
115.90	198.0
116.80	317.0
117.90	233.0
119.00	283.0
128.00	204.0
130.00	217.0
140.90	438.0
142.90	643.0
145.00	178.0
147.80	109.0
155.00	170.0
171.90	731.0
174.00	39888.0
175.00	3323.0
176.00	38552.0
176.90	2511.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44