

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080124\
 Data File : VU060287.D
 Acq On : 01 Aug 2024 10:05
 Operator : MD/SY
 Sample : VU0801MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Quant Time: Aug 02 02:32:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 02 02:32:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	219486	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	220691	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	86168	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	85812	60.892	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 121.780%			
7) Chloroethane-d5	1.904	69	66091	55.756	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 111.520%			
11) 1,1-Dichloroethene-d2	2.560	63	99999	39.942	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 79.880%			
21) 2-Butanone-d5	4.615	46	105944	108.175	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 108.180%			
24) Chloroform-d	5.052	84	136953	50.184	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.360%			
26) 1,2-Dichloroethane-d4	5.695	65	82793	51.023	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.040%			
32) Benzene-d6	5.718	84	276450	48.918	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 97.840%			
36) 1,2-Dichloropropane-d6	6.682	67	94031	53.761	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 107.520%			
41) Toluene-d8	7.891	98	229932	42.784	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 85.560%			
43) trans-1,3-Dichloroprop...	8.174	79	37786	46.168	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 92.340%			
47) 2-Hexanone-d5	8.627	63	59130	80.218	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 80.220%			
56) 1,1,2,2-Tetrachloroeth...	10.749	84	136094	50.695	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 101.380%			
66) 1,2-Dichlorobenzene-d4	12.187	152	78545	49.605	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.200%			
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	9177	5.595	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080124\
Data File : VU060287.D
Acq On : 01 Aug 2024 10:05
Operator : MD/SY
Sample : VU0801MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Time: Aug 02 02:32:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 02 02:32:23 2024
Response via : Initial Calibration

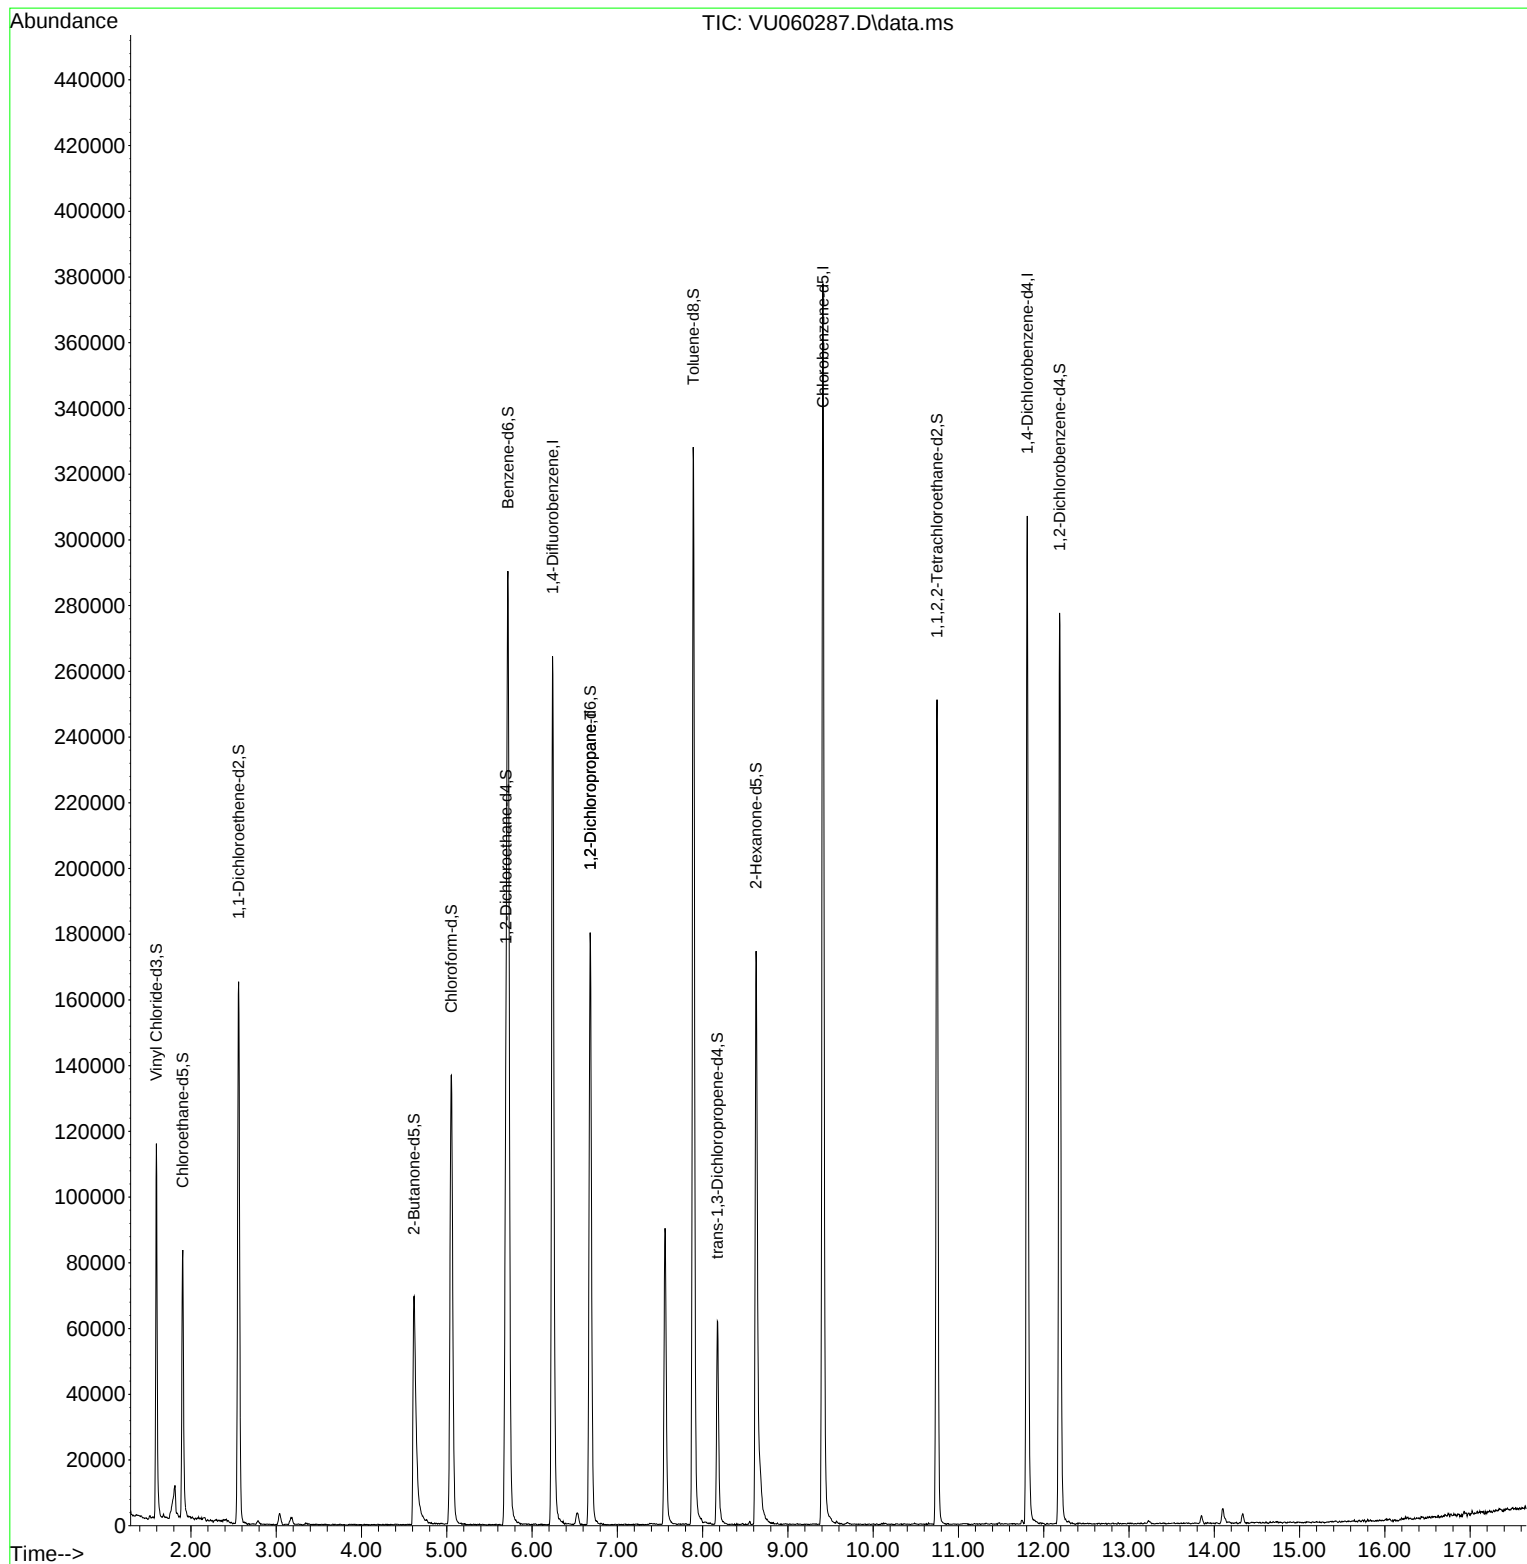

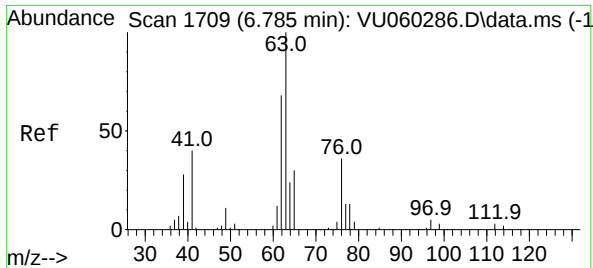

#37
 1,2-Dichloropropane
 Concen: 5.595 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.103 min
 Lab File: VU060287.D
 Acq: 01 Aug 2024 10:05

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Tgt Ion: 63 Resp: 9177
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.6#

