

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080124\
 Data File : VU060288.D
 Acq On : 01 Aug 2024 10:28
 Operator : MD/SY
 Sample : VU0801WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Quant Time: Aug 02 02:33:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 02 02:32:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	214220	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	222139	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	85354	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	81121	58.978	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 117.960%			
7) Chloroethane-d5	1.901	69	64474	55.729	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 111.460%			
11) 1,1-Dichloroethene-d2	2.557	63	94628	38.726	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.460%			
21) 2-Butanone-d5	4.615	46	105656	110.533	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 110.530%			
24) Chloroform-d	5.052	84	129823	48.740	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 97.480%			
26) 1,2-Dichloroethane-d4	5.692	65	81741	51.613	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.220%			
32) Benzene-d6	5.718	84	268185	47.147	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 94.300%			
36) 1,2-Dichloropropane-d6	6.682	67	91683	52.077	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 104.160%			
41) Toluene-d8	7.891	98	220220	40.710	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 81.420%			
43) trans-1,3-Dichloroprop...	8.174	79	37352	45.340	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 90.680%			
47) 2-Hexanone-d5	8.624	63	60008	80.878	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 80.880%			
56) 1,1,2,2-Tetrachloroeth...	10.747	84	131770	48.764	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 97.520%			
66) 1,2-Dichlorobenzene-d4	12.187	152	79901	50.942	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 101.880%			
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	9216	5.582	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080124\
Data File : VU060288.D
Acq On : 01 Aug 2024 10:28
Operator : MD/SY
Sample : VU0801WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Time: Aug 02 02:33:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 02 02:32:23 2024
Response via : Initial Calibration

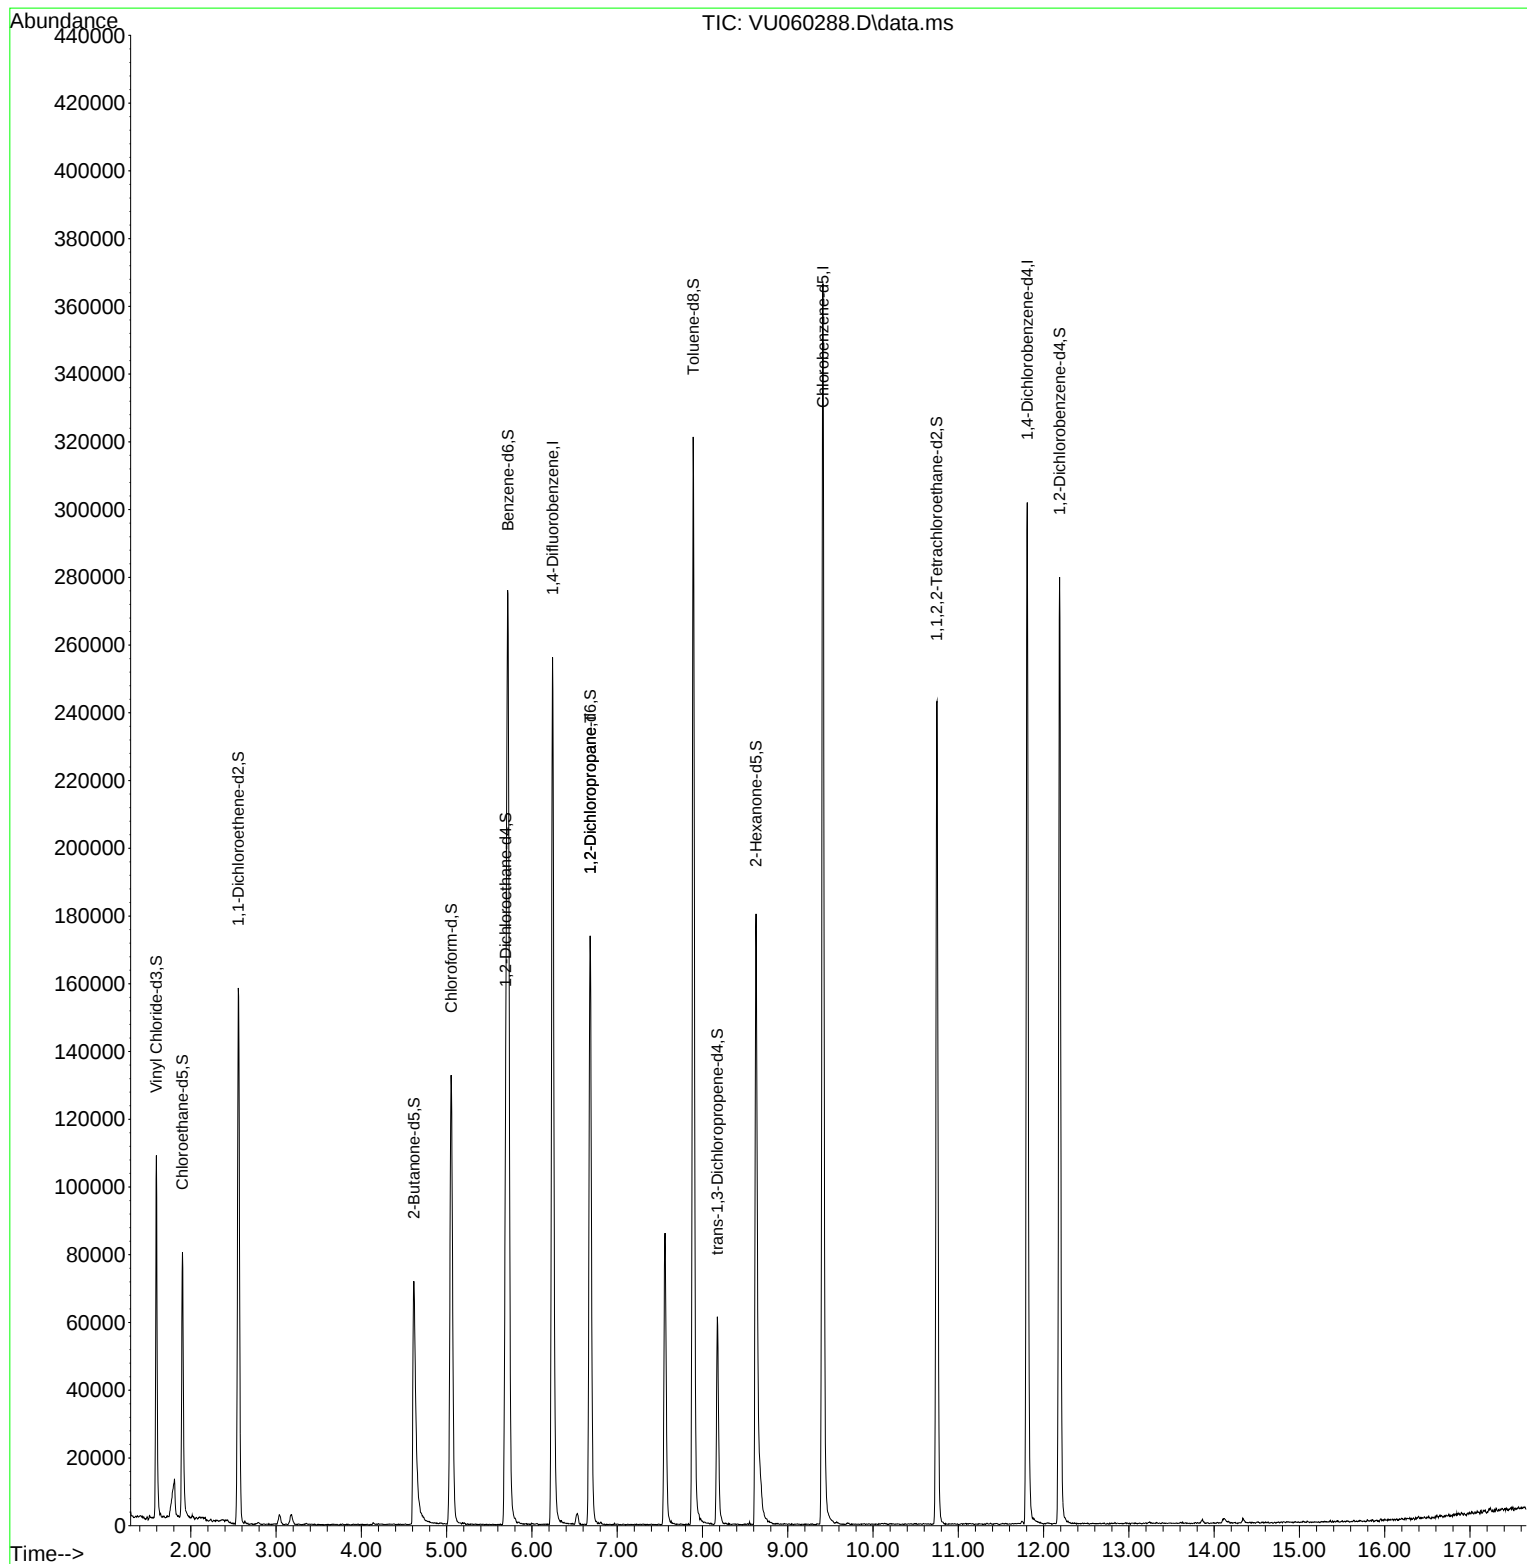

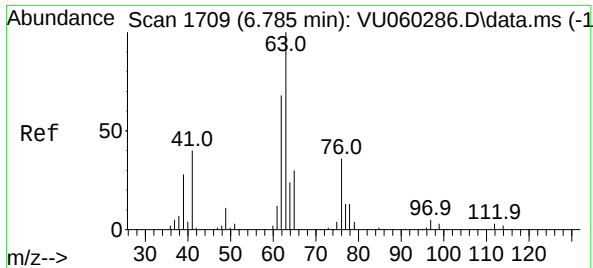

#37
 1,2-Dichloropropane
 Concen: 5.582 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.103 min
 Lab File: VU060288.D
 Acq: 01 Aug 2024 10:28

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Tgt Ion: 63 Resp: 9216
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.6#

