
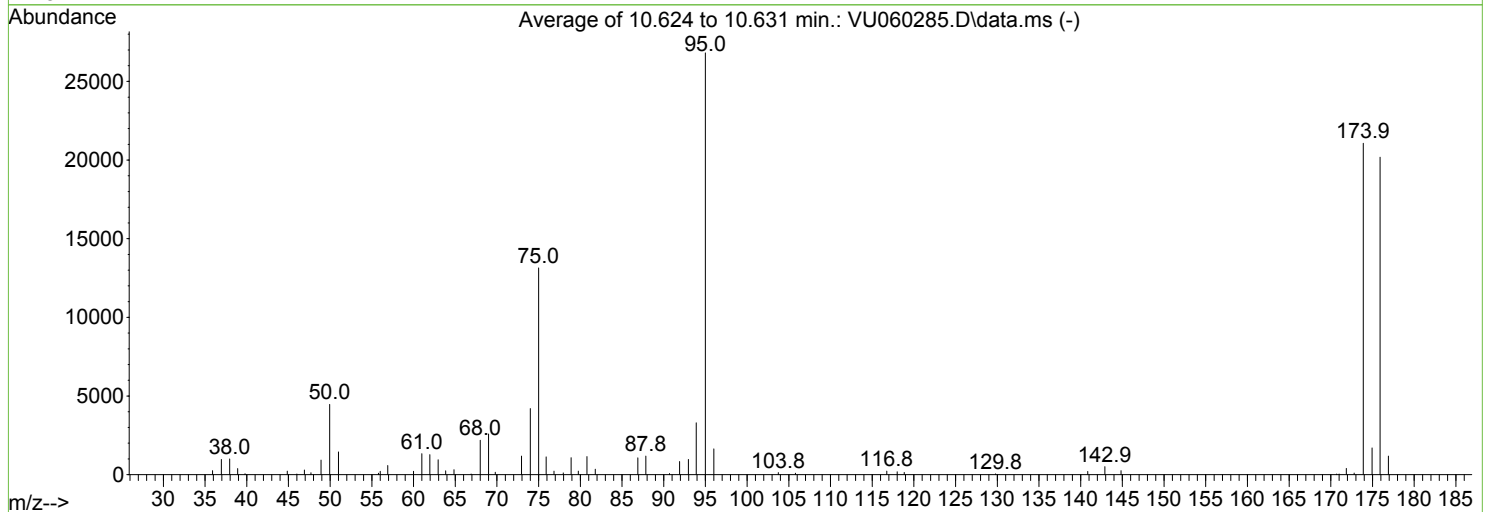


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080124\
Data File : VU060285.D
Acq On : 01 Aug 2024 08:47
Operator : MD/SY
Sample : BFB076
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB076

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Fri Aug 02 02:32:23 2024

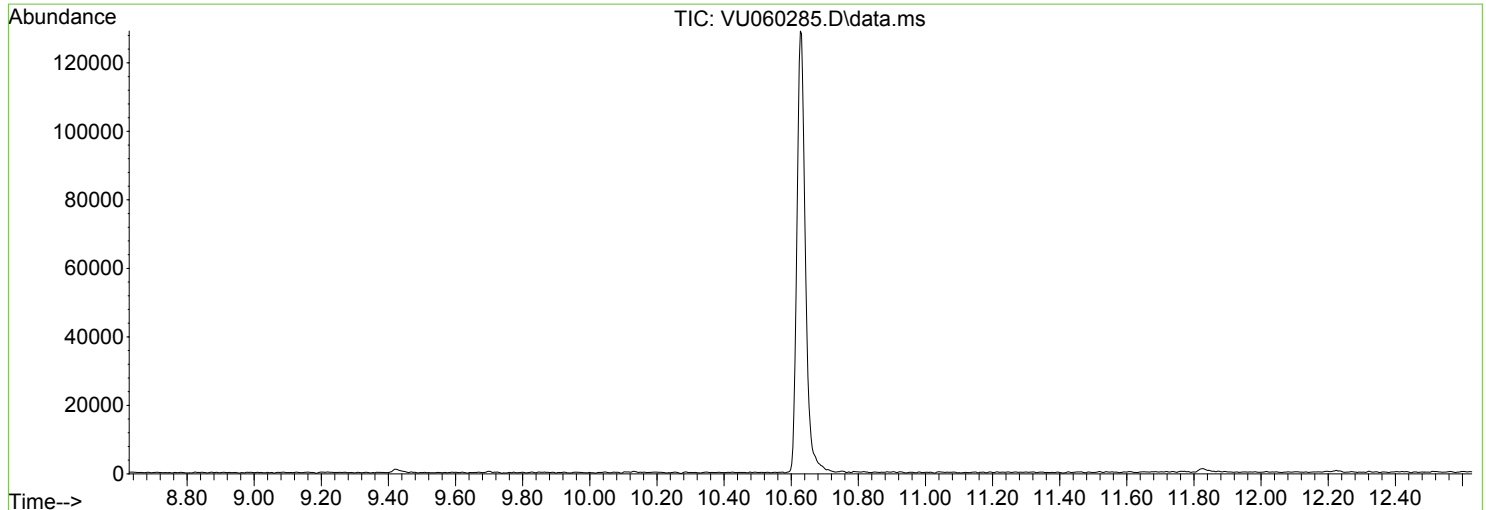

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	4471	PASS
75	95	30	80	49.0	13146	PASS
95	95	100	100	100.0	26816	PASS
96	95	5	9	6.1	1637	PASS
173	174	0.00	2	0.5	103	PASS
174	95	50	120	78.6	21072	PASS
175	174	5	9	8.1	1697	PASS
176	174	95	101	95.8	20184	PASS
177	176	5	9	5.9	1183	PASS

m/z	Abundance
35.90	187.0
37.00	1044.0
37.90	982.0
38.90	391.0
39.80	187.0
43.90	326.0
44.80	213.0
46.90	319.0
47.70	101.0
48.90	904.0
49.90	4482.0
51.00	1400.0
55.80	285.0
56.90	491.0
60.00	207.0
61.00	1281.0
61.90	1178.0
62.90	839.0
63.80	229.0
64.80	282.0
66.90	122.0
68.00	2078.0
69.00	2461.0
69.80	171.0
73.00	1192.0
74.00	4106.0
75.00	12589.0
75.90	1154.0
76.80	261.0
78.90	1038.0
79.70	201.0
80.80	1043.0
81.80	321.0
86.90	1073.0
87.80	1195.0
91.90	787.0
92.90	1007.0
93.90	3331.0
95.00	25832.0
96.00	1443.0
103.70	125.0
116.70	177.0
118.00	156.0
118.80	139.0
140.90	221.0
142.90	436.0
144.90	237.0
171.80	359.0
173.90	19640.0
175.00	1662.0
175.90	19248.0
176.90	1058.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	281.0
37.00	991.0
38.00	1031.0
38.90	399.0
39.80	193.0
43.80	309.0
44.80	235.0
46.90	306.0
47.70	128.0
48.90	937.0
50.00	4539.0
51.00	1482.0
56.00	301.0
56.90	590.0
60.00	232.0
61.00	1400.0
62.00	1297.0
62.90	969.0
63.90	234.0
64.80	330.0
68.00	2225.0
69.00	2658.0
69.80	161.0
72.90	1217.0
74.00	4332.0
75.00	13529.0
75.90	1159.0
76.90	252.0
78.00	139.0
78.90	1109.0
79.70	235.0
80.80	1190.0
81.80	347.0
86.90	1073.0
87.90	1186.0
90.70	105.0
91.90	874.0
93.00	943.0
93.90	3468.0
95.00	27680.0
96.00	1657.0
103.70	150.0
105.80	114.0
116.70	233.0
118.00	199.0
118.80	135.0
140.80	197.0
142.90	523.0
144.90	255.0
171.80	411.0
173.90	21664.0
175.00	1797.0
175.90	20672.0
176.90	1193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	289.0
36.90	851.0
38.00	975.0
38.90	360.0
39.80	179.0
43.90	361.0
44.90	218.0
46.00	109.0
46.90	273.0
47.70	149.0
48.90	926.0
50.00	4391.0
51.00	1460.0
56.00	341.0
56.90	659.0
60.00	207.0
61.00	1316.0
62.00	1328.0
63.00	1028.0
63.90	256.0
64.90	323.0
68.00	2245.0
69.00	2643.0
69.80	131.0
72.90	1125.0
74.00	4171.0
75.00	13319.0
75.90	1082.0
76.90	171.0
77.90	186.0
78.90	1083.0
79.80	231.0
80.80	1213.0
81.80	386.0
86.90	1053.0
87.90	1157.0
90.70	112.0
91.90	828.0
93.00	953.0
93.90	3079.0
95.00	26936.0
96.00	1811.0
103.80	114.0
105.80	148.0
116.80	274.0
118.00	184.0
118.90	165.0
129.80	149.0
140.80	205.0
142.90	561.0
144.80	263.0
170.70	124.0
171.00	126.0
171.90	411.0
172.80	310.0
173.90	21912.0
174.90	1633.0
175.90	20632.0
176.90	1298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
39.80	122.0
43.90	376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076