

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080218\
 Data File : VU025793.D
 Acq On : 02 Aug 2018 12:40
 Operator : MD/SY
 Sample : J4205-01RE
 Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JJ1K8RE

Quant Time: Aug 03 04:29:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 04:24:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	674940	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	652925	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	389654	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	87677	22.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	45.50%#
7) Chloroethane-d5	1.64	69	48724	15.33	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	30.66%#
11) 1,1-Dichloroethene-d2	2.24	63	137341	17.12	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	34.24%#
21) 2-Butanone-d5	4.19	46	197191	66.29	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	66.29%
24) Chloroform-d	4.65	84	225782	26.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	52.62%#
26) 1,2-Dichloroethane-d4	5.31	65	160037	28.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	56.38%#
32) Benzene-d6	5.34	84	431714	25.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	51.56%#
36) 1,2-Dichloropropane-d6	6.33	67	144089	26.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	53.40%#
41) Toluene-d8	7.57	98	410196	25.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	51.08%#
43) trans-1,3-Dichloropropene-	7.85	79	72891	26.45	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	52.90%#
47) 2-Hexanone-d5	8.33	63	152469	67.49	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.49%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	232591	30.82	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	61.64%#
64) 1,2-Dichlorobenzene-d4	11.87	152	208330	26.38	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	52.76%#


Target Compounds					Ovalue
37) 1,2-Dichloropropane	6.33	63	16571	3.23 ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080218\
Data File : VU025793.D
Acq On : 02 Aug 2018 12:40
Operator : MD/SY
Sample : J4205-01RE
Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JJ1K8RE

Quant Time: Aug 03 04:29:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 03 04:24:02 2018
Response via : Initial Calibration

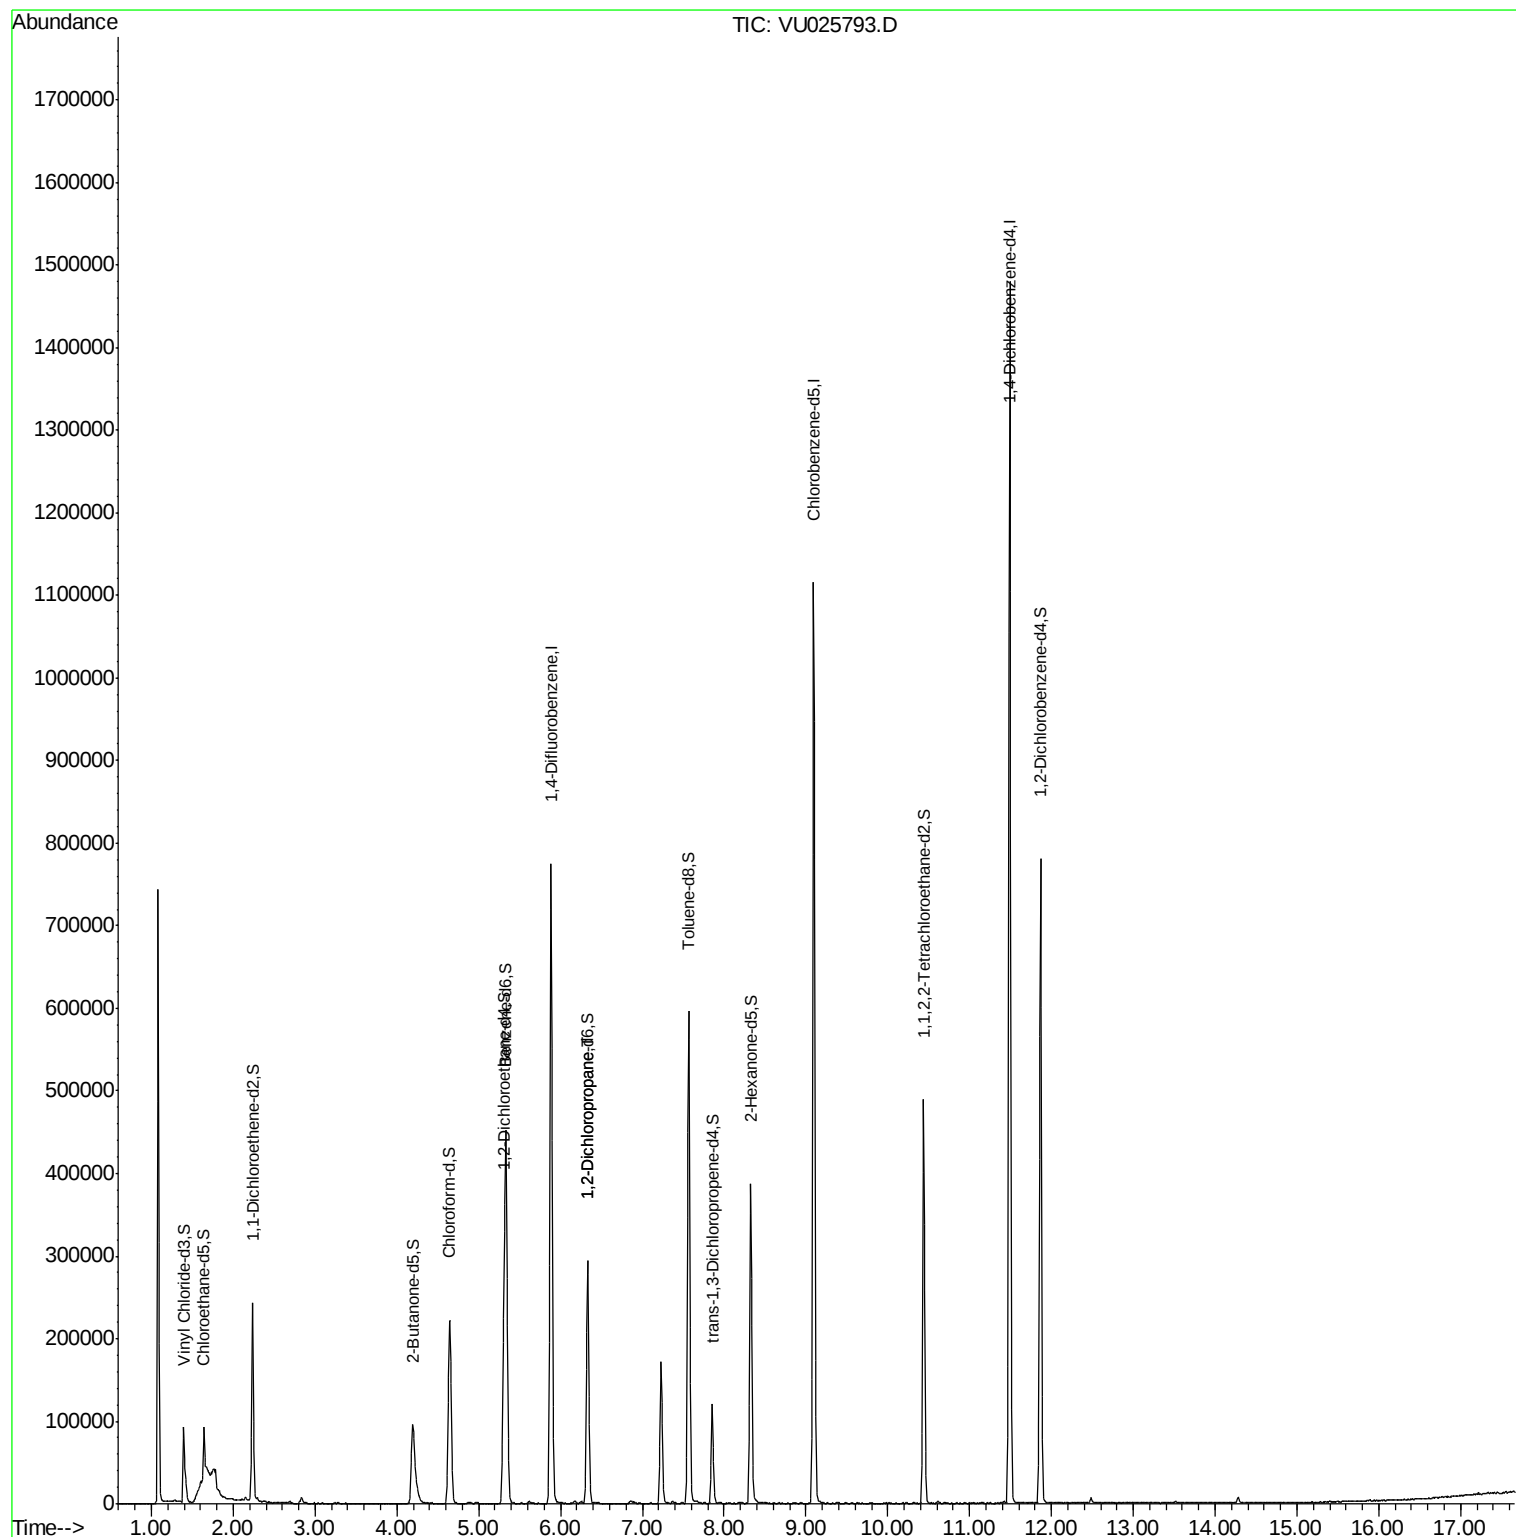

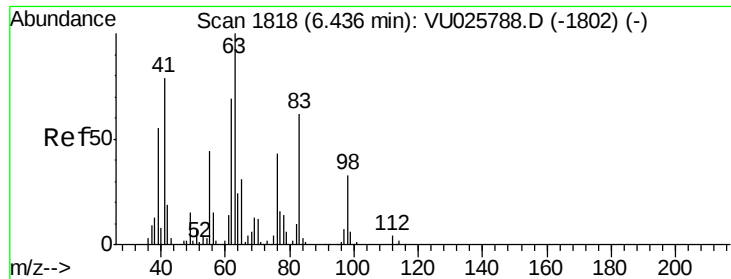

#37
 1,2-Dichloropropane
 Concen: 3.23 ug/L
 RT: 6.33 min Scan# 1786
 Delta R.T. -0.10 min
 Lab File: VU025793.D
 Acq: 02 Aug 2018 12:40

Instrument :
 MSVOA_U
 ClientSampleId :
 JJ1K8RE

Tot Ion: 63 Resp: 16571
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.3 4.9#

