

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080218\
 Data File : VU025798.D
 Acq On : 02 Aug 2018 17:40
 Operator : MD/SY
 Sample : J4265-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Aug 03 05:57:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 03 05:43:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	353502	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	333032	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	170961	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	79325	39.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.62%
7) Chloroethane-d5	1.68	69	62863	37.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.52%
11) 1,1-Dichloroethene-d2	2.27	63	121744	28.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.96%#
21) 2-Butanone-d5	4.18	46	127584	81.89	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.89%
24) Chloroform-d	4.65	84	165545	36.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.66%
26) 1,2-Dichloroethane-d4	5.31	65	116122	39.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.12%
32) Benzene-d6	5.35	84	329543	38.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.16%
36) 1,2-Dichloropropane-d6	6.34	67	105742	38.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	76.84%
41) Toluene-d8	7.57	98	312396	38.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.28%#
43) trans-1,3-Dichloropropene-	7.85	79	53815	38.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.56%
47) 2-Hexanone-d5	8.31	63	93117	80.80	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.80%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	142860	37.11	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.22%
64) 1,2-Dichlorobenzene-d4	11.86	152	132917	38.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.72%#


Target Compounds					Ovalue
13) Acetone	2.32	43	4921	2.69 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080218\
Data File : VU025798.D
Acq On : 02 Aug 2018 17:40
Operator : MD/SY
Sample : J4265-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Aug 03 05:57:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 03 05:43:06 2018
Response via : Initial Calibration

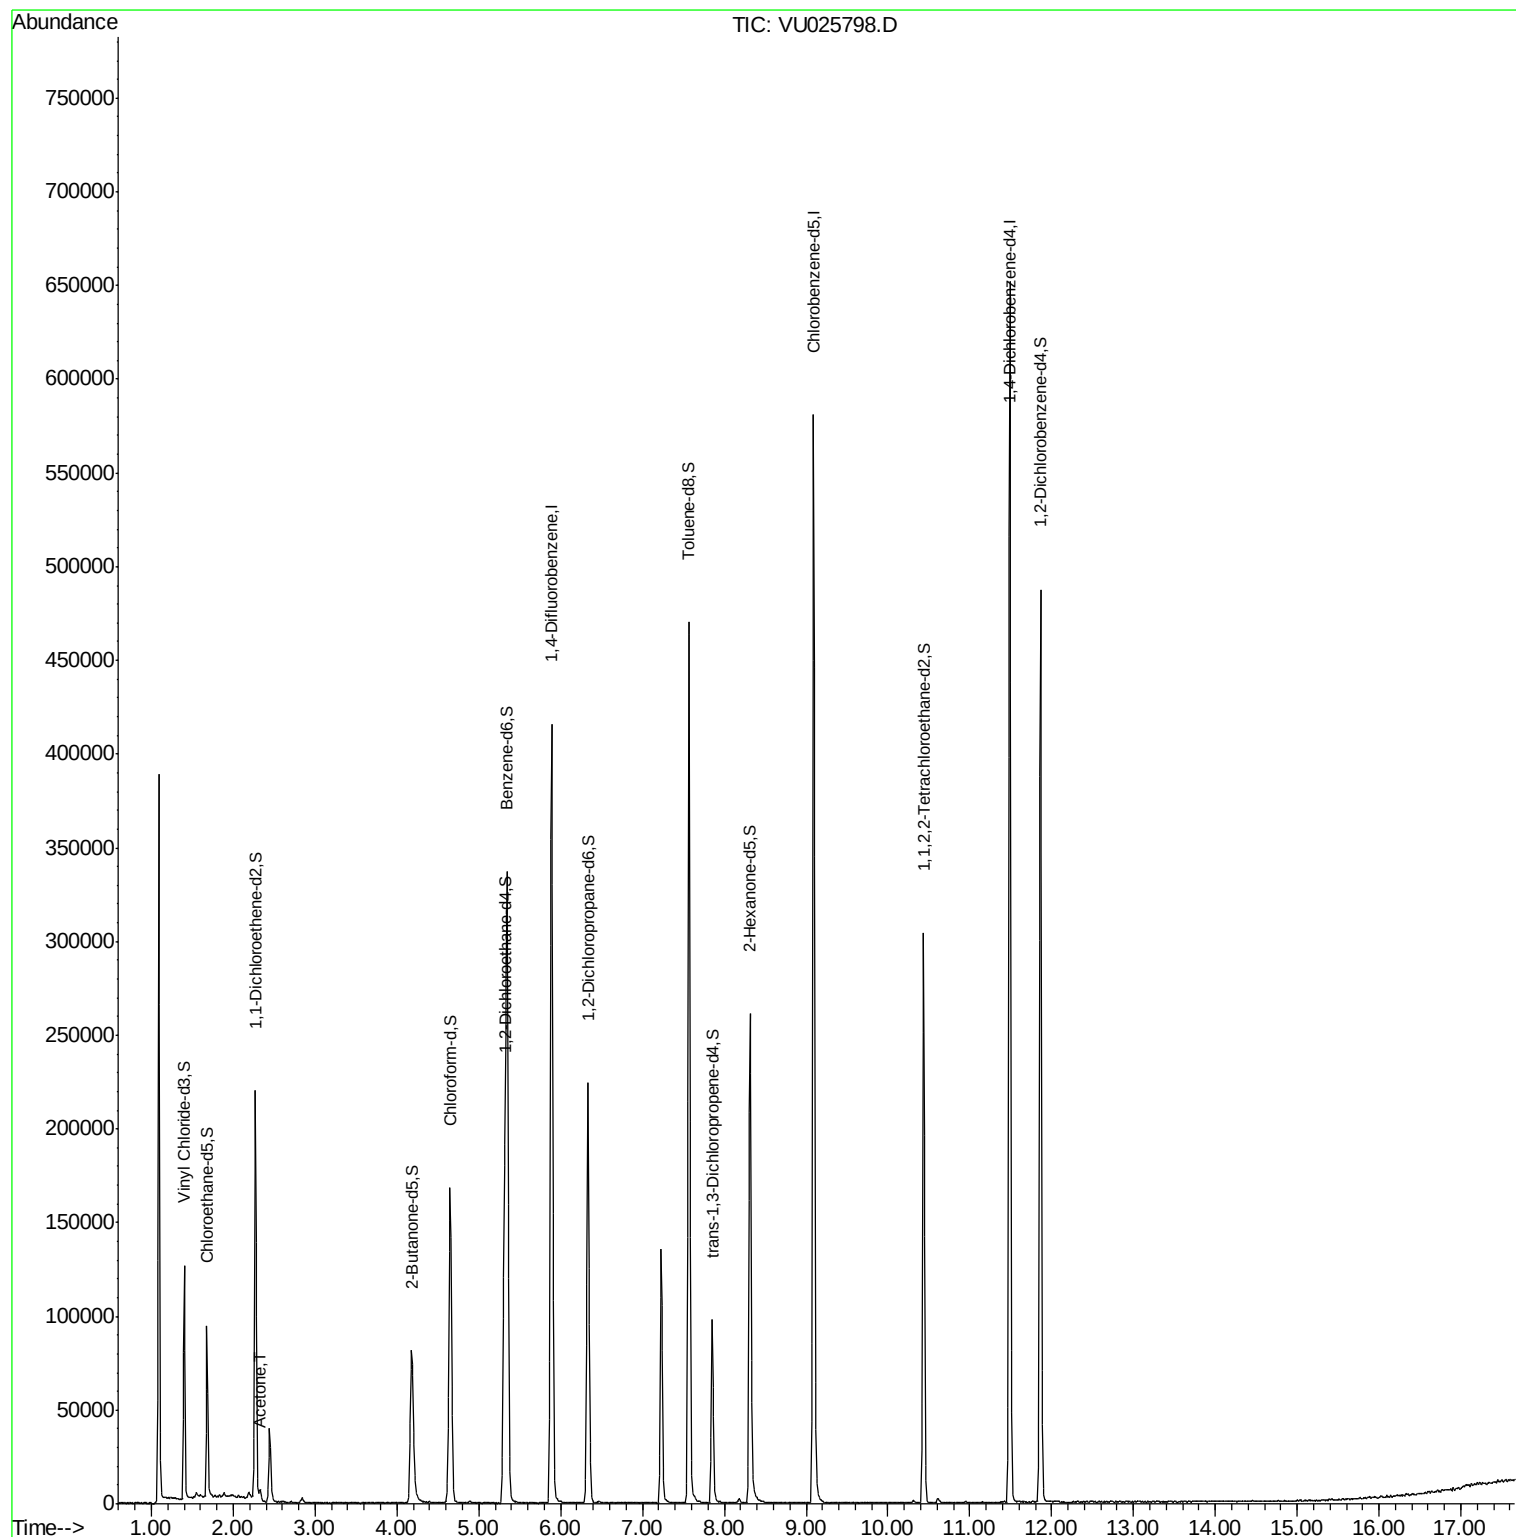

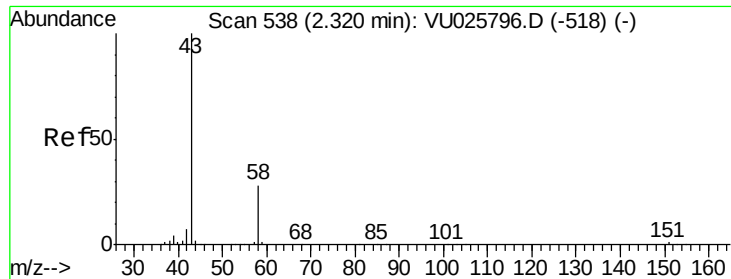

#13
 Acetone
 Concen: 2.69 ug/L
 RT: 2.32 min Scan# 539
 Delta R.T. 0.00 min
 Lab File: VU025798.D
 Acq: 02 Aug 2018 17:40

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Tot Ion: 43 Resp: 4921
 Ion Ratio Lower Upper
 43 100
 58 26.1 0.0 61.2

