


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080218\
 Data File : VU025787.D
 Acq On : 02 Aug 2018 09:09
 Operator : MD/SY
 Sample : BFB52
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB52

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 06 01:30:36 2018

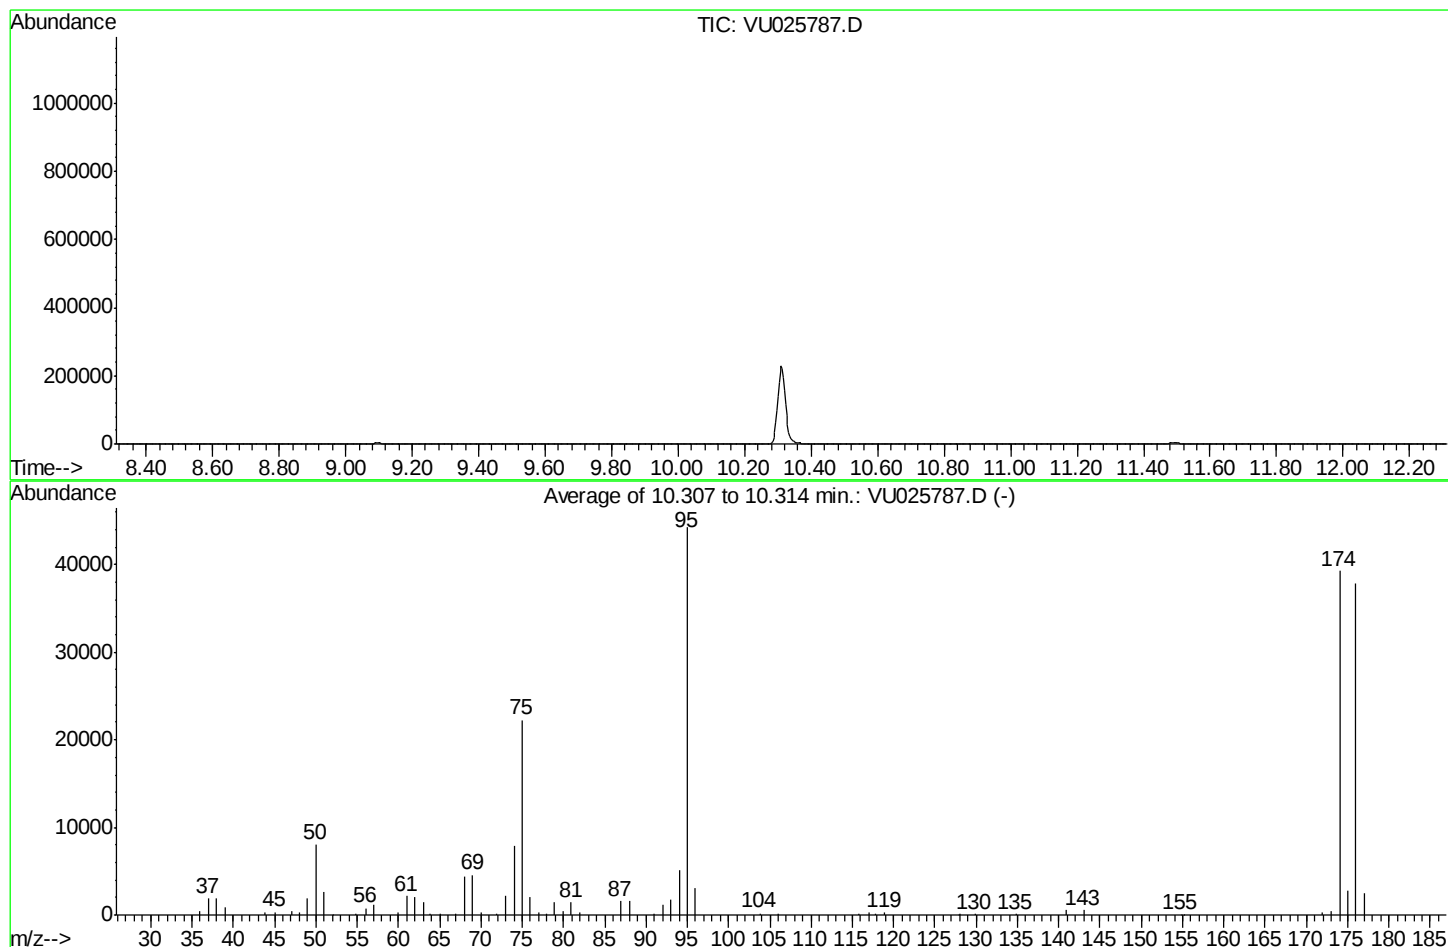

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8030	PASS
75	95	30	80	50.3	22250	PASS
95	95	100	100	100.0	44250	PASS
96	95	5	9	7.1	3130	PASS
173	174	0.00	2	1.2	474	PASS
174	95	50	120	88.7	39242	PASS
175	174	5	9	7.2	2824	PASS
176	174	95	101	96.4	37829	PASS
177	176	5	9	6.6	2493	PASS

Scan 3011 (10.272 min): VU025787.D
BFB52

m/z	Abundance
40.10	154.0
43.90	333.0
207.00	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	478.0
37.00	1928.0
38.00	1824.0
39.00	936.0
40.00	152.0
43.90	628.0
45.00	280.0
47.10	466.0
48.00	302.0
49.00	1725.0
50.00	7845.0
51.00	2642.0
52.00	121.0
54.90	165.0
56.10	693.0
57.00	1117.0
59.90	342.0
61.00	2017.0
62.00	1906.0
63.00	1452.0
63.90	159.0
65.10	208.0
67.10	135.0
68.00	4383.0
69.00	4640.0
70.00	431.0
71.90	200.0
73.00	2116.0
74.00	7817.0
75.00	22008.0
76.00	1962.0
77.00	230.0
78.00	160.0
78.90	1435.0
79.90	394.0
80.90	1417.0
81.90	265.0
86.90	1434.0
87.90	1619.0
90.90	158.0
92.00	1327.0
93.00	1776.0
94.00	5061.0
95.00	42464.0
96.00	3101.0
103.90	191.0
106.00	154.0
115.80	229.0
117.00	272.0
117.80	212.0
118.90	257.0
127.80	102.0
129.80	143.0
134.80	150.0
140.90	538.0
143.00	479.0
155.10	104.0
171.90	188.0
173.00	480.0
174.00	37040.0
175.00	2762.0
176.00	35648.0
176.90	2506.0
207.00	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	471.0
37.00	1923.0
38.00	1871.0
39.00	921.0
40.00	142.0
43.90	585.0
45.10	358.0
47.10	448.0
48.00	285.0
49.00	1934.0
50.00	8236.0
51.00	2714.0
54.90	182.0
56.10	753.0
57.00	1196.0
59.90	302.0
61.00	2254.0
62.00	2089.0
63.00	1478.0
63.90	183.0
65.10	205.0
67.00	151.0
68.00	4495.0
69.00	4688.0
70.00	334.0
71.90	211.0
73.00	2198.0
74.00	8181.0
75.00	22768.0
76.00	2025.0
77.00	286.0
78.00	192.0
78.90	1563.0
80.00	442.0
80.90	1474.0
81.90	280.0
86.90	1571.0
87.90	1597.0
90.80	142.0
92.00	1245.0
93.00	1809.0
94.00	5286.0
95.00	45976.0
96.00	3229.0
103.80	193.0
106.00	139.0
115.80	198.0
117.00	258.0
117.80	212.0
119.00	290.0
128.00	118.0
129.90	141.0
134.90	136.0
140.90	564.0
143.00	556.0
154.80	105.0
171.90	216.0
173.00	491.0
174.00	40424.0
175.00	2939.0
176.00	39072.0
177.00	2613.0
207.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
35.90	412.0
37.00	1846.0
38.00	1846.0
39.00	819.0
40.00	147.0
43.90	529.0
45.10	394.0
47.10	347.0
48.00	256.0
49.00	1911.0
50.00	8010.0
51.00	2469.0
54.90	171.0
56.00	770.0
57.00	1125.0
60.00	287.0
61.00	2221.0
62.00	2050.0
63.00	1337.0
63.90	200.0
65.00	164.0
66.90	156.0
68.00	4260.0
69.00	4340.0
70.00	278.0
72.00	189.0
73.00	2137.0
74.00	7523.0
75.00	21976.0
76.00	2009.0
77.00	299.0
78.00	190.0
78.90	1496.0
80.00	472.0
80.90	1421.0
81.90	309.0
86.90	1704.0
88.00	1480.0
91.00	151.0
92.00	1147.0
93.00	1751.0
94.00	4892.0
95.00	44312.0
96.00	3061.0
103.70	144.0
105.90	122.0
115.90	193.0
117.00	267.0
117.90	211.0
119.00	283.0
128.00	125.0
129.90	156.0
134.90	116.0
140.90	528.0
143.00	608.0
154.80	103.0
171.90	290.0
173.00	452.0
174.00	40264.0
175.00	2773.0
176.00	38768.0
176.90	2360.0
207.10	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52