

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080219\
 Data File : VU033575.D
 Acq On : 02 Aug 2019 17:15
 Operator : JC/SP
 Sample : K4103-18DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9F9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.174	23	26	34	rVB	3195	2749	0.23%	0.029%
2	1.389	86	93	106	rVB	189312	200122	16.97%	2.079%
3	1.672	173	181	196	rVB	150308	188380	15.97%	1.957%
4	2.257	352	363	376	rVB	286764	435441	36.92%	4.524%
5	2.453	421	424	426	rBV3	487	319	0.03%	0.003%
6	2.546	450	453	457	rBV	313	219	0.02%	0.002%
7	2.682	486	495	504	rBV4	1183	2008	0.17%	0.021%
8	2.730	506	510	511	rVV2	487	369	0.03%	0.004%
9	2.739	511	513	517	rVB2	362	186	0.02%	0.002%
10	2.775	522	524	526	rBV	403	244	0.02%	0.003%
11	2.820	526	538	553	rVB2	6079	12489	1.06%	0.130%
12	3.273	676	679	682	rBV2	825	686	0.06%	0.007%
13	3.508	750	752	758	rVB	398	301	0.03%	0.003%
14	3.585	772	776	781	rVB2	166	186	0.02%	0.002%
15	4.000	903	905	910	rVB2	307	276	0.02%	0.003%
16	4.151	939	952	962	rBV	109748	285751	24.23%	2.969%
17	4.402	1027	1030	1036	rBV2	446	404	0.03%	0.004%
18	4.620	1080	1098	1120	rBV	198533	466495	39.56%	4.847%
19	4.816	1155	1159	1164	rBV2	362	433	0.04%	0.004%
20	4.932	1192	1195	1199	rBV2	395	314	0.03%	0.003%
21	4.971	1204	1207	1211	rVB2	253	181	0.02%	0.002%
22	5.032	1219	1226	1227	rBV2	271	206	0.02%	0.002%
23	5.070	1236	1238	1246	rVB3	302	364	0.03%	0.004%
24	5.180	1269	1272	1274	rBV3	342	190	0.02%	0.002%
25	5.318	1291	1315	1340	rBV2	401615	1179353	100.00%	12.253%
26	5.537	1380	1383	1386	rBV2	358	227	0.02%	0.002%
27	5.566	1389	1392	1395	rVB2	389	225	0.02%	0.002%
28	5.649	1413	1418	1422	rBV3	455	444	0.04%	0.005%
29	5.765	1447	1454	1463	rVB5	1754	3149	0.27%	0.033%
30	5.865	1470	1485	1506	rBV	346128	677151	57.42%	7.035%
31	6.164	1564	1578	1606	rBV	216362	425475	36.08%	4.420%
32	6.308	1609	1623	1646	rVV	263168	527067	44.69%	5.476%
33	6.521	1683	1689	1690	rBV	399	329	0.03%	0.003%
34	6.623	1719	1721	1724	rVV2	302	197	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080219\
 Data File : VU033575.D
 Acq On : 02 Aug 2019 17:15
 Operator : JC/SP
 Sample : K4103-18DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9F9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

35	6.652	1724	1730	1732	rVV2	190	233	0.02%	0.002%
36	6.804	1773	1777	1783	rVB3	426	358	0.03%	0.004%
37	6.865	1792	1796	1799	rVV	282	236	0.02%	0.002%
38	6.961	1821	1826	1830	rBV	173	198	0.02%	0.002%
39	7.209	1886	1903	1935	rBV	143548	262151	22.23%	2.724%
40	7.331	1936	1941	1946	rVB4	793	879	0.07%	0.009%
41	7.402	1960	1963	1969	rVB2	566	632	0.05%	0.007%
42	7.546	1994	2008	2029	rBV	529601	924194	78.36%	9.602%
43	7.832	2082	2097	2115	rBV	103068	180572	15.31%	1.876%
44	7.955	2133	2135	2142	rVB3	444	363	0.03%	0.004%
45	8.019	2152	2155	2158	rVB	389	253	0.02%	0.003%
46	8.167	2191	2201	2205	rBV4	1283	1753	0.15%	0.018%
47	8.295	2229	2241	2268	rBV	352989	615399	52.18%	6.394%
48	8.453	2286	2290	2301	rVB6	3155	5072	0.43%	0.053%
49	8.566	2323	2325	2329	rVB2	292	179	0.02%	0.002%
50	8.594	2332	2334	2340	rVB3	328	273	0.02%	0.003%
51	8.659	2352	2354	2358	rVB2	424	239	0.02%	0.002%
52	8.713	2368	2371	2377	rVB2	418	323	0.03%	0.003%
53	8.784	2389	2393	2397	rVB4	224	247	0.02%	0.003%
54	8.810	2397	2401	2404	rBV	275	178	0.02%	0.002%
55	8.836	2404	2409	2412	rBV2	292	227	0.02%	0.002%
56	8.929	2434	2438	2442	rBV	239	200	0.02%	0.002%
57	9.074	2470	2483	2515	rBV	515302	868978	73.68%	9.028%
58	9.234	2531	2533	2538	rVB2	339	220	0.02%	0.002%
59	9.286	2545	2549	2554	rBV4	383	286	0.02%	0.003%
60	9.334	2562	2564	2569	rVB3	268	208	0.02%	0.002%
61	9.360	2569	2572	2576	rBV2	485	322	0.03%	0.003%
62	9.382	2576	2579	2583	rVB2	281	195	0.02%	0.002%
63	9.427	2585	2593	2601	rVB5	4397	6546	0.56%	0.068%
64	9.501	2612	2616	2620	rBV2	375	295	0.03%	0.003%
65	9.594	2637	2645	2648	rBV2	180	262	0.02%	0.003%
66	9.659	2661	2665	2669	rVB2	301	229	0.02%	0.002%
67	9.688	2669	2674	2676	rBV2	336	246	0.02%	0.003%
68	9.774	2699	2701	2706	rBV2	252	186	0.02%	0.002%
69	9.938	2749	2752	2756	rVB3	334	240	0.02%	0.002%
70	10.019	2769	2777	2789	rVV4	2986	5057	0.43%	0.053%
71	10.064	2789	2791	2796	rVV2	210	205	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080219\
 Data File : VU033575.D
 Acq On : 02 Aug 2019 17:15
 Operator : JC/SP
 Sample : K4103-18DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB9F9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
 Title : VOC Analysis

72	10.324	2866	2872	2874	rBV2	280	265	0.02%	0.003%
73	10.414	2886	2900	2922	rVV	391566	632092	53.60%	6.567%
74	10.504	2925	2928	2931	rVV4	439	383	0.03%	0.004%
75	10.524	2931	2934	2938	rVV	397	415	0.04%	0.004%
76	10.543	2938	2940	2945	rVB	513	306	0.03%	0.003%
77	10.591	2950	2955	2963	rBV6	1675	2168	0.18%	0.023%
78	10.723	2992	2996	2997	rBV2	505	315	0.03%	0.003%
79	10.733	2997	2999	3011	rVB3	828	895	0.08%	0.009%
80	10.800	3014	3020	3025	rVB5	1697	1850	0.16%	0.019%
81	10.845	3030	3034	3039	rBV2	398	361	0.03%	0.004%
82	10.864	3039	3040	3048	rVB	217	195	0.02%	0.002%
83	10.919	3053	3057	3059	rVB	282	193	0.02%	0.002%
84	11.263	3162	3164	3168	rVB2	528	281	0.02%	0.003%
85	11.315	3176	3180	3182	rBV2	343	213	0.02%	0.002%
86	11.363	3188	3195	3201	rBV7	2531	3883	0.33%	0.040%
87	11.469	3216	3228	3248	rBV	515043	818934	69.44%	8.508%
88	11.665	3285	3289	3294	rBV3	438	446	0.04%	0.005%
89	11.845	3332	3345	3366	rBV	533631	866077	73.44%	8.998%
90	12.189	3447	3452	3457	rBV4	541	689	0.06%	0.007%
91	12.340	3496	3499	3502	rBV2	331	215	0.02%	0.002%
92	12.607	3579	3582	3584	rBV	644	490	0.04%	0.005%
93	12.768	3630	3632	3640	rVB3	496	528	0.04%	0.005%
94	12.803	3640	3643	3648	rBV3	399	409	0.03%	0.004%
95	13.032	3708	3714	3723	rBV5	1597	2896	0.25%	0.030%
96	13.440	3837	3841	3843	rBV2	488	385	0.03%	0.004%
97	13.504	3858	3861	3863	rVB3	353	178	0.02%	0.002%
98	13.588	3885	3887	3889	rBV2	348	202	0.02%	0.002%
99	14.253	4092	4094	4096	rBV2	333	180	0.02%	0.002%
100	14.388	4134	4136	4140	rBV2	504	284	0.02%	0.003%


Sum of corrected areas: 9625292

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080219\
Data File : VU033575.D
Acq On : 02 Aug 2019 17:15
Operator : JC/SP
Sample : K4103-18DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9F9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

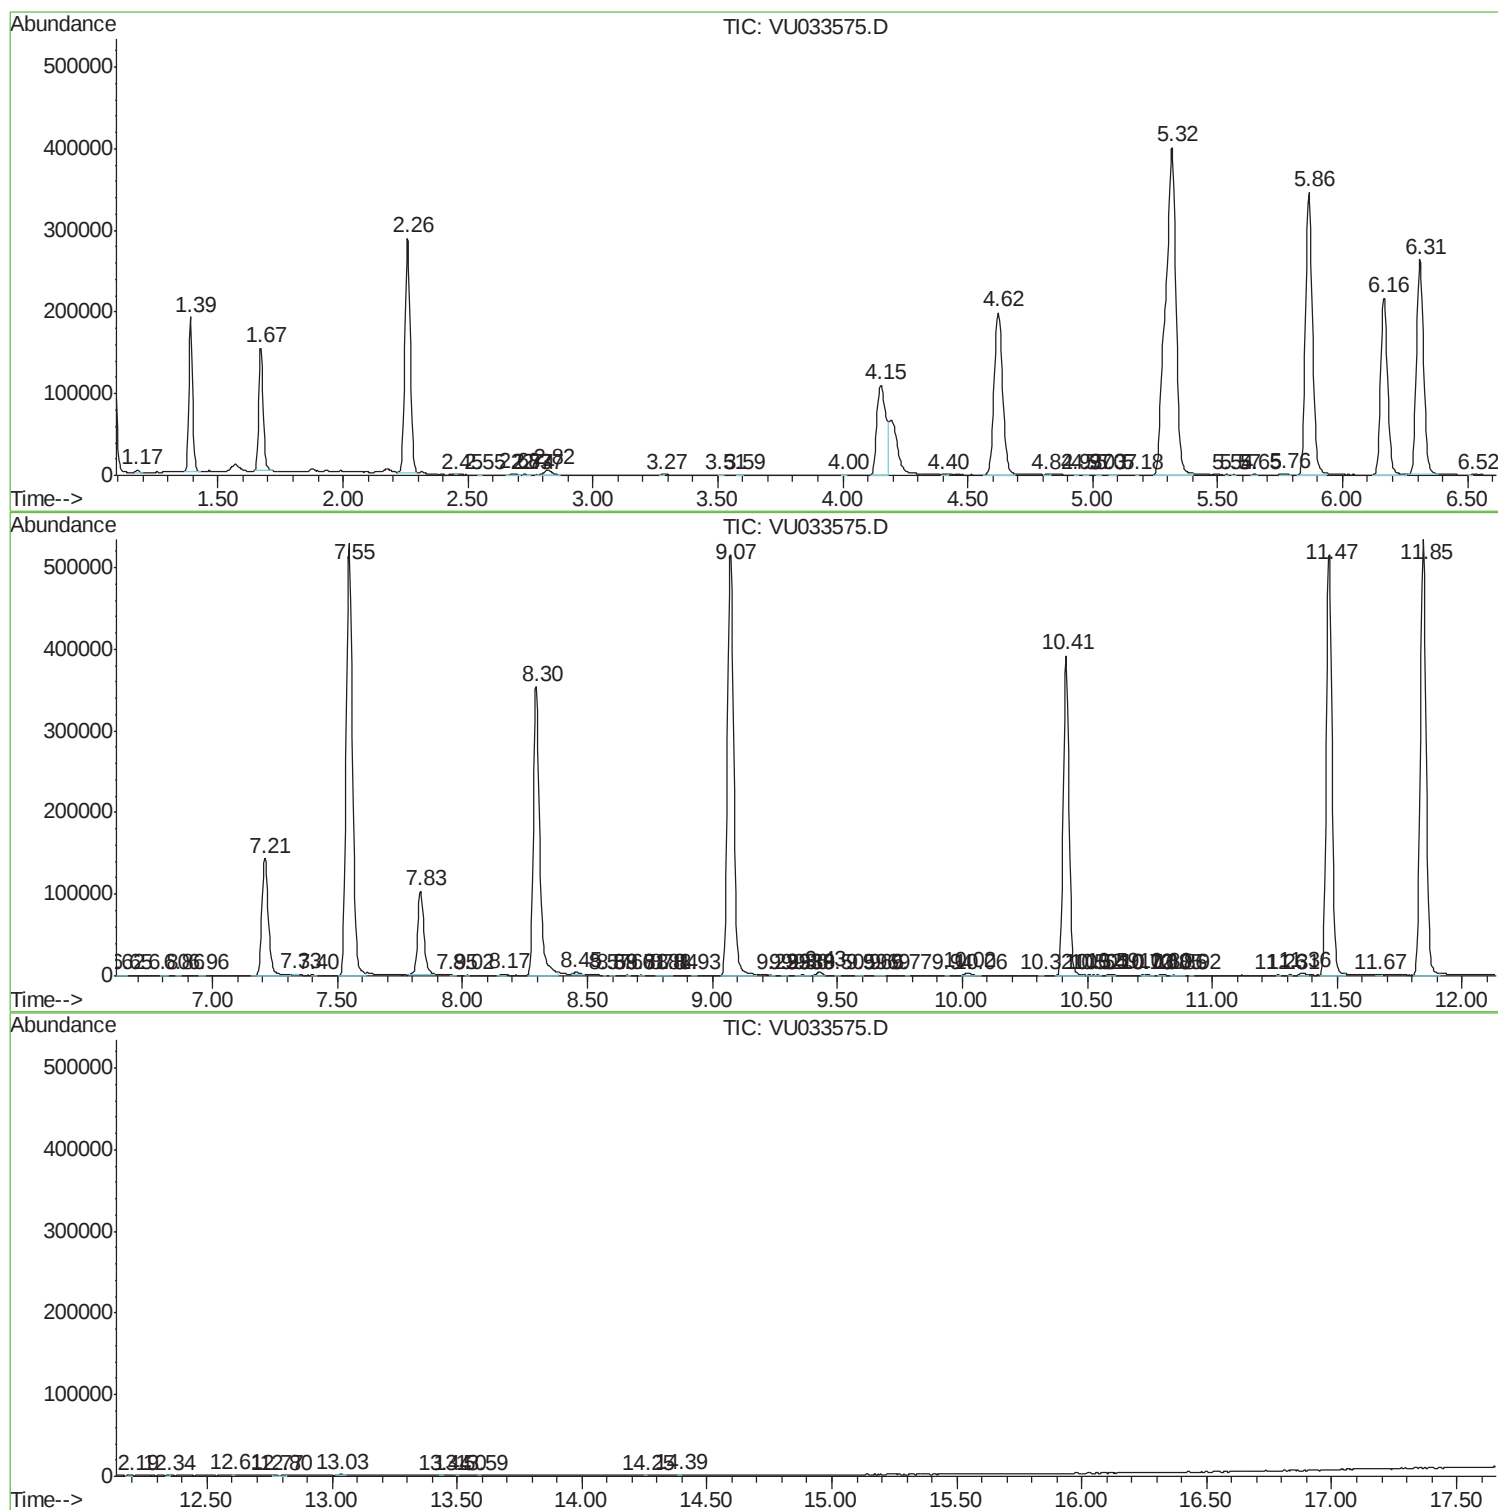

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU080219\
Data File : VU033575.D
Acq On : 02 Aug 2019 17:15
Operator : JC/SP
Sample : K4103-18DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9F9DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080219\
Data File : VU033575.D
Acq On : 02 Aug 2019 17:15
Operator : JC/SP
Sample : K4103-18DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB9F9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc