


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080219\
Data File : VU033556.D
Acq On : 02 Aug 2019 08:22
Operator : JC/SP
Sample : BFB45
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM073119WMA.M
Title : VOC Analysis
Last Update : Sat Aug 03 00:39:04 2019

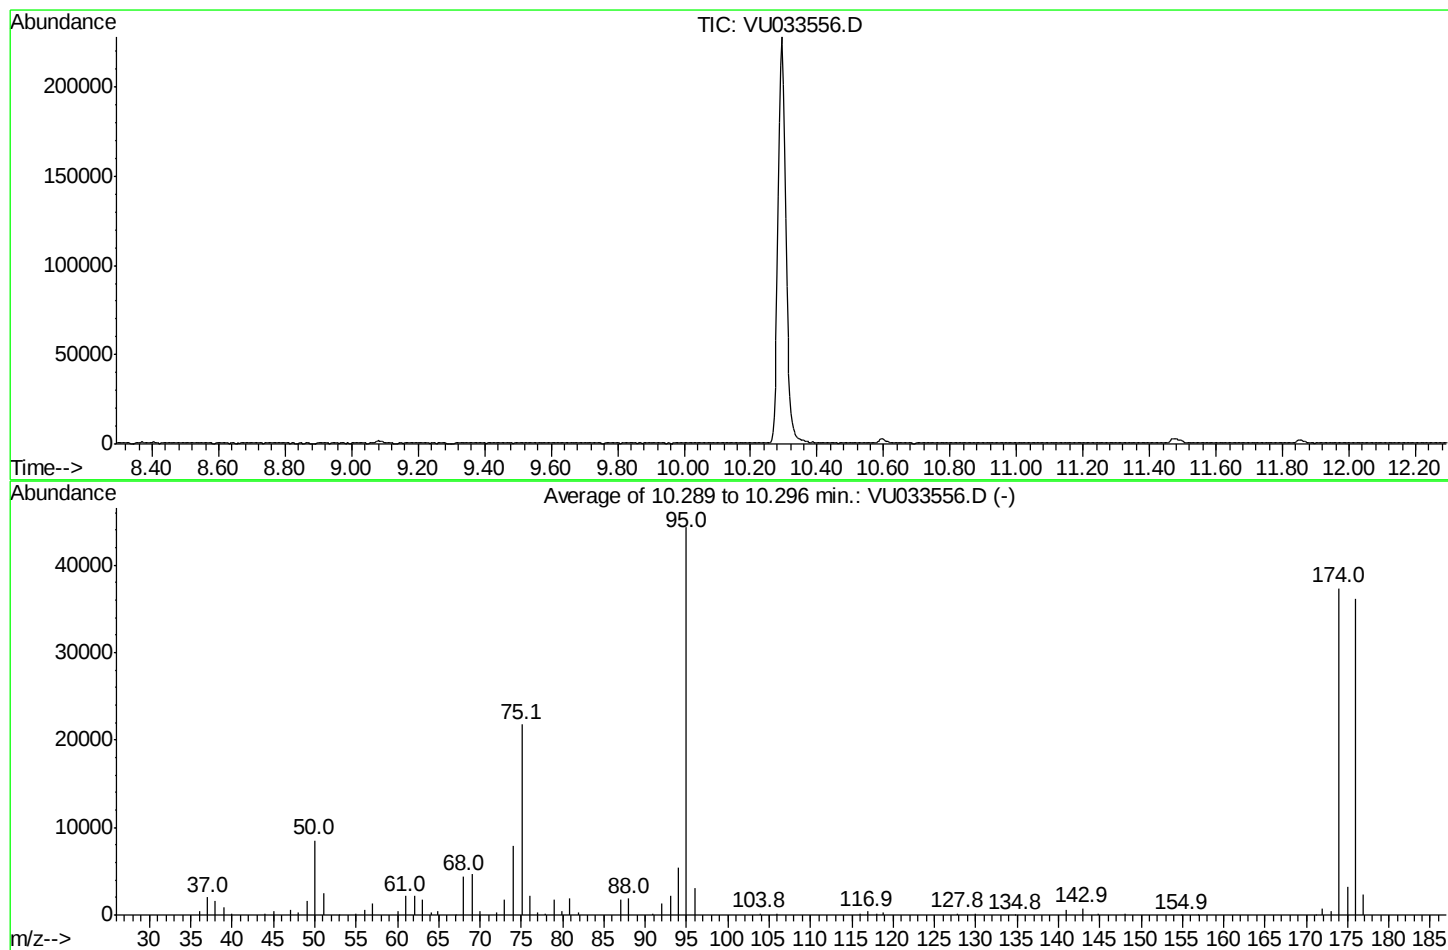

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	8505	PASS
75	95	30	80	49.1	21770	PASS
95	95	100	100	100.0	44301	PASS
96	95	5	9	6.9	3042	PASS
173	174	0.00	2	1.3	481	PASS
174	95	50	120	84.2	37314	PASS
175	174	5	9	8.5	3187	PASS
176	174	95	101	96.9	36152	PASS
177	176	5	9	6.4	2309	PASS

Scan 2850 (10.254 min): VU033556.D
BFB45

m/z	Abundance
39.90	138.0
44.00	332.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	507.0
37.00	1804.0
38.00	1700.0
39.00	872.0
39.90	240.0
43.90	458.0
45.00	381.0
47.00	561.0
48.00	256.0
49.00	1608.0
50.00	8293.0
51.10	2203.0
53.00	109.0
54.90	141.0
56.00	626.0
57.00	1324.0
60.10	411.0
61.00	2119.0
62.10	2091.0
63.00	1596.0
64.00	241.0
65.00	476.0
67.00	147.0
68.00	4256.0
69.00	4529.0
70.00	447.0
72.00	314.0
73.00	1708.0
74.00	7769.0
75.10	20952.0
76.00	1986.0
77.00	272.0
77.90	165.0
78.90	1650.0
80.00	389.0
80.90	1803.0
81.90	301.0
87.00	1677.0
88.00	1873.0
90.90	166.0
92.00	1349.0
93.00	2111.0
94.00	5492.0
95.00	42736.0
96.00	3163.0
103.80	216.0
105.90	163.0
116.00	120.0
116.90	336.0
117.90	192.0
118.80	320.0
127.80	183.0
129.90	108.0
134.80	111.0
140.90	475.0
142.90	731.0
144.90	200.0
148.00	130.0
154.90	116.0
171.10	101.0
171.90	627.0
173.00	683.0
174.00	34856.0
174.90	3028.0
176.00	33936.0
176.90	2198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	539.0
37.00	2130.0
38.00	1726.0
39.00	909.0
39.90	223.0
44.00	504.0
45.00	384.0
47.00	607.0
47.90	226.0
49.00	1681.0
50.00	8767.0
51.00	2520.0
54.90	165.0
56.00	612.0
57.00	1367.0
60.10	435.0
61.00	2258.0
62.10	2270.0
63.00	1777.0
64.00	261.0
64.90	448.0
68.00	4654.0
69.00	4786.0
70.00	458.0
72.00	304.0
73.00	1848.0
74.00	8129.0
75.10	22512.0
76.00	2252.0
77.00	330.0
77.90	208.0
78.90	1756.0
80.00	425.0
80.90	1934.0
81.90	350.0
87.00	1823.0
88.00	1953.0
90.80	201.0
92.00	1380.0
93.00	2299.0
94.00	5653.0
95.00	45520.0
96.00	3056.0
103.90	233.0
105.90	154.0
116.00	153.0
116.90	403.0
118.00	188.0
118.80	327.0
127.80	185.0
129.90	113.0
140.90	550.0
142.90	762.0
144.90	196.0
148.00	177.0
154.90	104.0
156.90	106.0
171.90	786.0
173.10	761.0
174.00	38432.0
175.00	3273.0
176.00	37040.0
177.00	2359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	459.0
37.00	2167.0
38.00	1637.0
39.00	934.0
39.90	219.0
44.00	596.0
45.00	405.0
47.00	623.0
47.90	230.0
49.00	1681.0
50.00	8456.0
51.00	2556.0
54.90	174.0
56.00	594.0
57.00	1303.0
60.00	400.0
61.00	2168.0
62.10	2228.0
63.00	1836.0
64.10	266.0
64.90	415.0
68.00	4397.0
69.00	4579.0
70.00	371.0
72.00	287.0
73.00	1810.0
74.00	7732.0
75.10	21848.0
76.00	2145.0
76.90	348.0
78.00	199.0
78.90	1689.0
79.90	413.0
80.90	1771.0
81.90	367.0
87.00	1757.0
88.00	1835.0
90.80	244.0
92.00	1282.0
93.00	2194.0
94.00	5253.0
95.00	44648.0
96.00	2907.0
103.90	222.0
105.90	150.0
115.90	213.0
116.90	396.0
118.00	168.0
118.90	290.0
127.80	176.0
129.90	134.0
140.90	547.0
142.90	732.0
144.80	188.0
148.00	177.0
171.90	831.0
174.00	38656.0
175.00	3260.0
176.00	37480.0
177.00	2370.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45