

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080318\
Data File : VU025813.D
Acq On : 03 Aug 2018 12:14
Operator : MD/SY
Sample : VU0803WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0803WBL01

Quant Time: Aug 04 05:37:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072518DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 27 15:10:58 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	31482	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	10195	0.87	ug/l	0.00
Spiked Amount	1.000		Recovery	=	87.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	11114	0.86	ug/l	0.00
Spiked Amount	1.000		Recovery	=	86.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080318\
Data File : VU025813.D
Acq On : 03 Aug 2018 12:14
Operator : MD/SY
Sample : VU0803WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0803WBL01

Quant Time: Aug 04 05:37:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U072518DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 27 15:10:58 2018
Response via : Initial Calibration

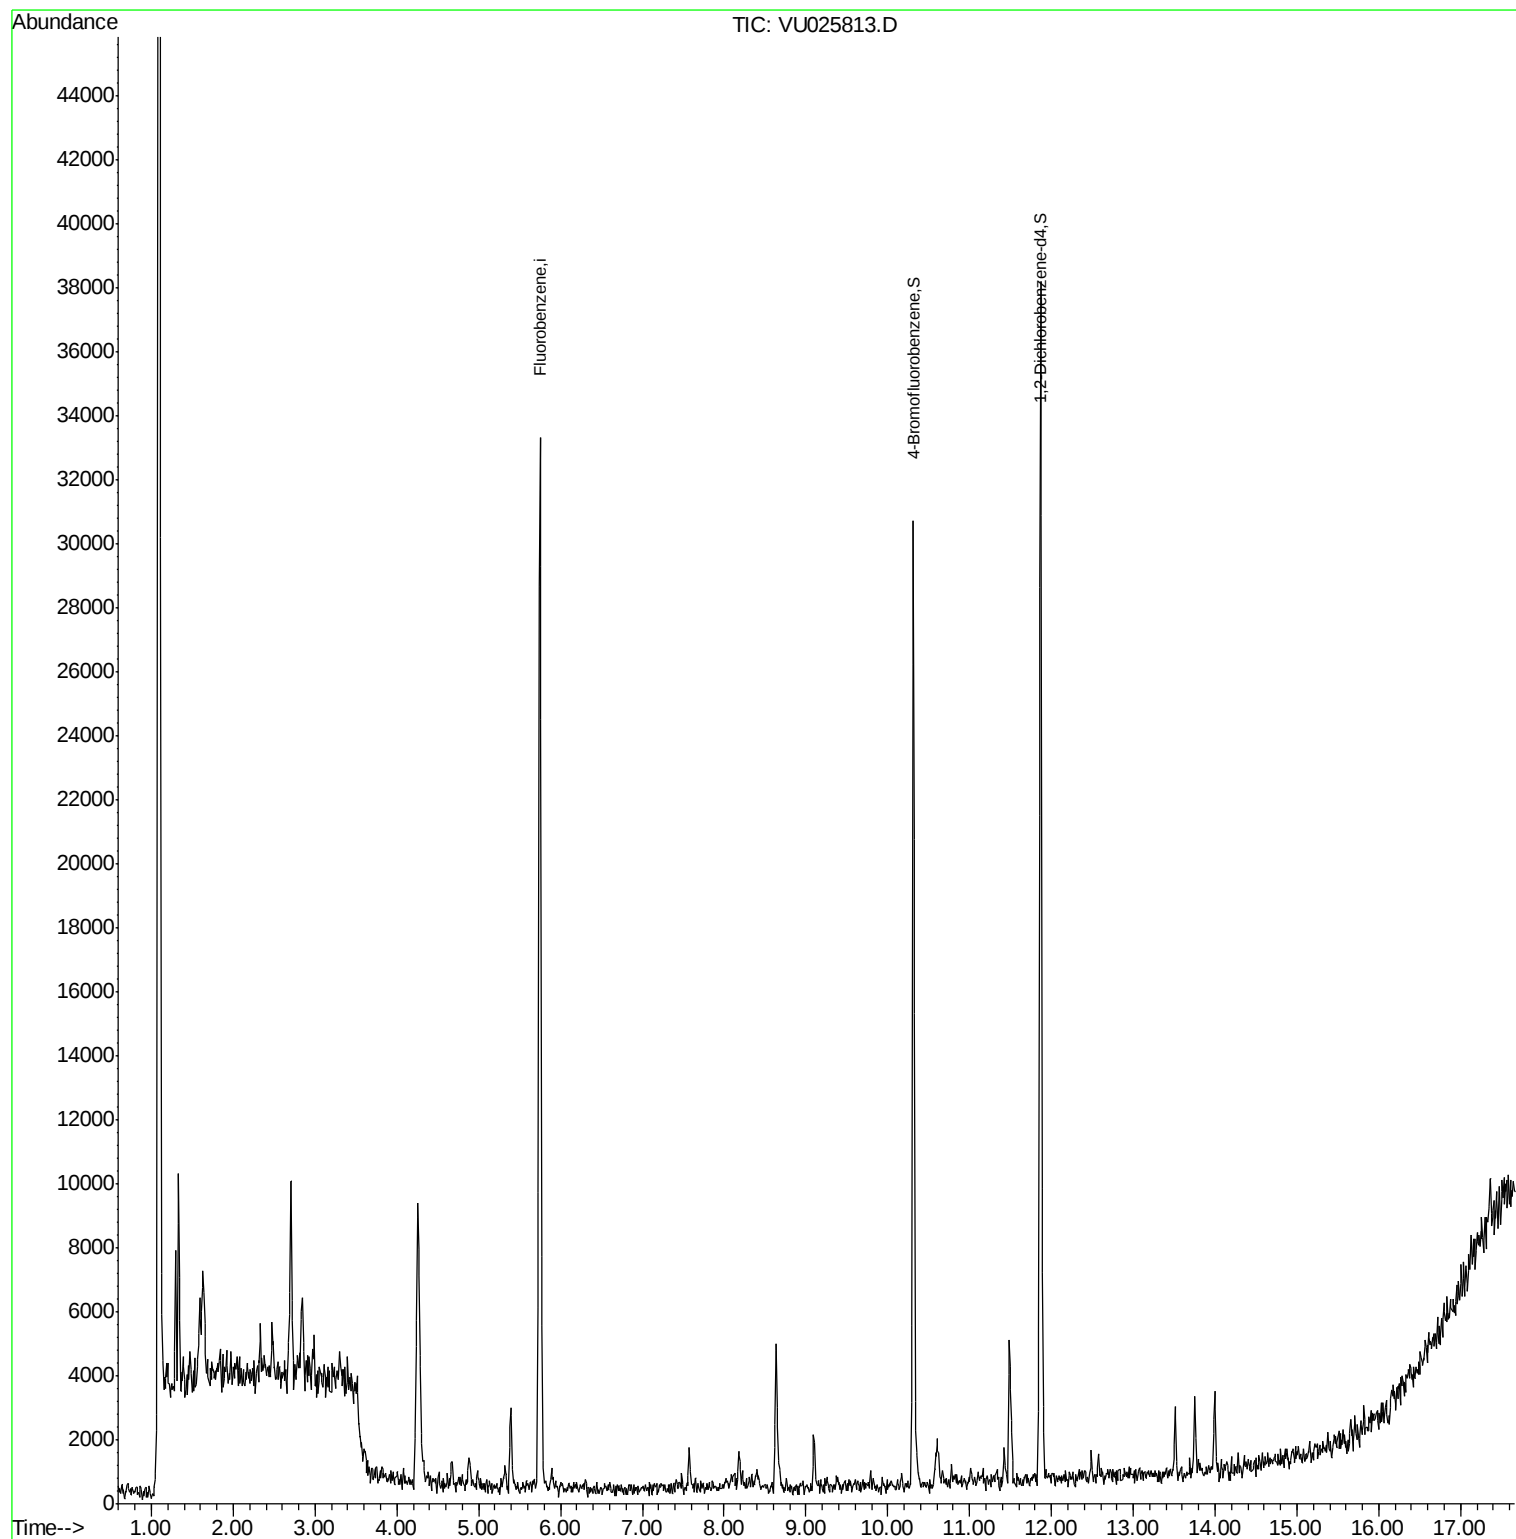

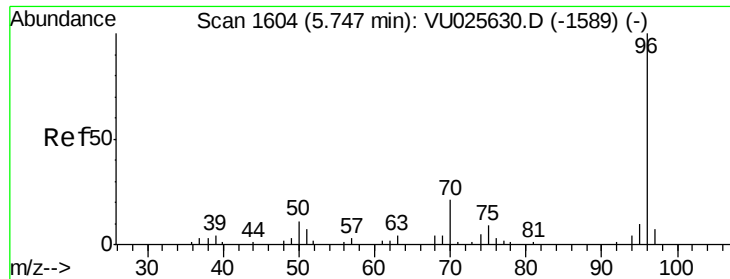

#1

Fluorobenzene

Concen: 1.00 ug/l

RT: 5.74 min Scan# 1603

Delta R.T. -0.00 min

Lab File: VU025813.D

Acq: 03 Aug 2018 12:14

Instrument :

MSVOA_U

ClientSampleId :

VU0803WBL01

Tot Ion: 96 Resp: 31482





Ion Ratio Lower Upper

96 100

70 20.3 16.2 24.4

95 9.4 6.9 10.3

97 6.1 0.0 0.0#

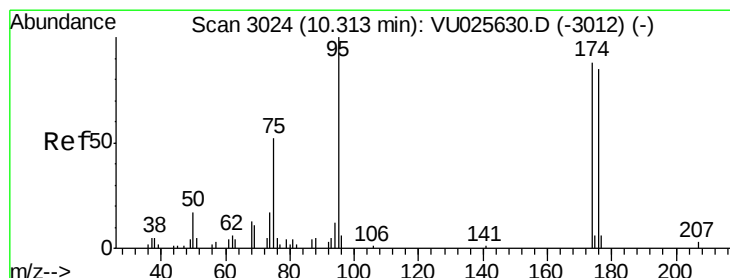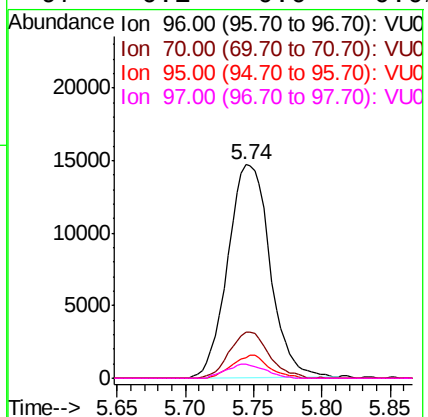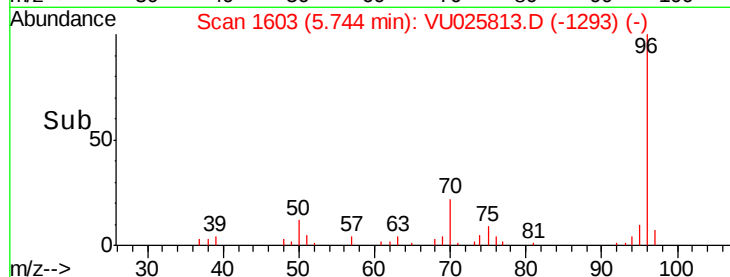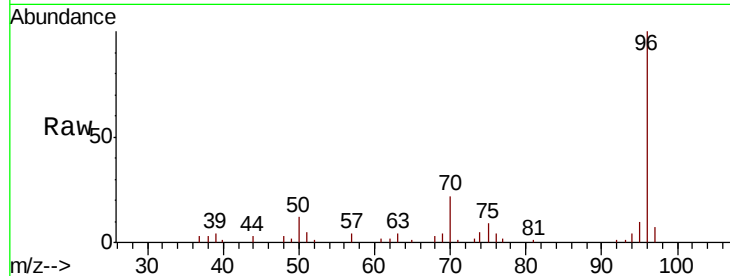

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 3024

Delta R.T. 0.00 min

Lab File: VU025813.D

Acq: 03 Aug 2018 12:14




Tgt Ion: 95 Resp: 10195


Ion Ratio Lower Upper

95 100

174 90.4 65.6 98.4

176 86.8 62.0 93.0

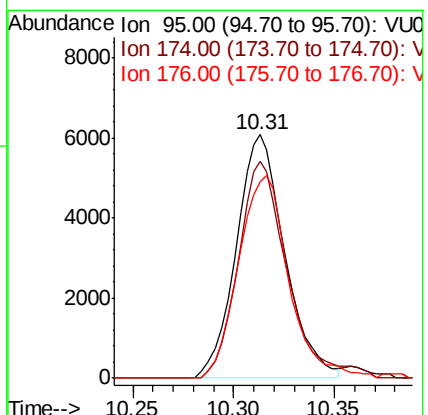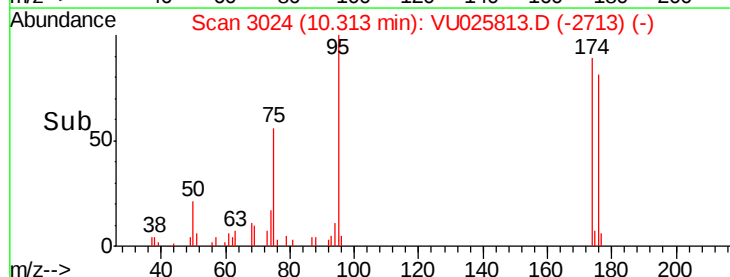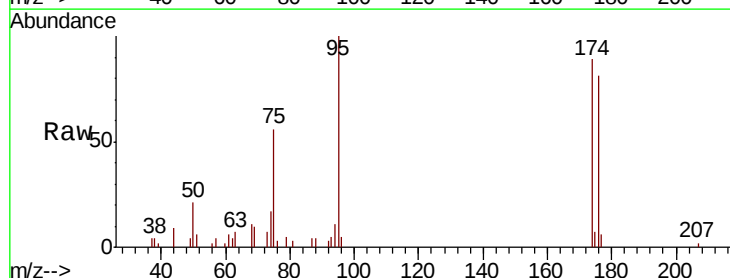

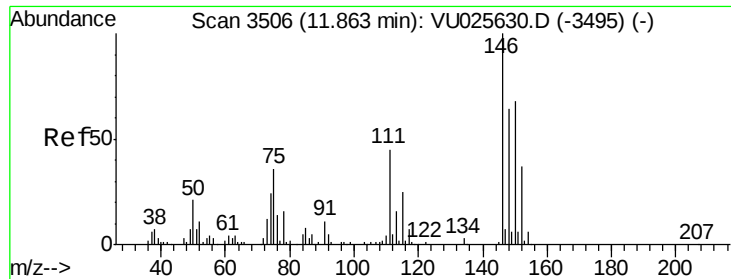

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3506
 Delta R.T. 0.00 min
 Lab File: VU025813.D
 Acq: 03 Aug 2018 12:14

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0803WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	62.1	0.0	118.8
150	156.8	0.0	0.0#

