


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080318\
 Data File : VU025811.D
 Acq On : 03 Aug 2018 11:04
 Operator : MD/SY
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072518DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jul 27 15:10:58 2018

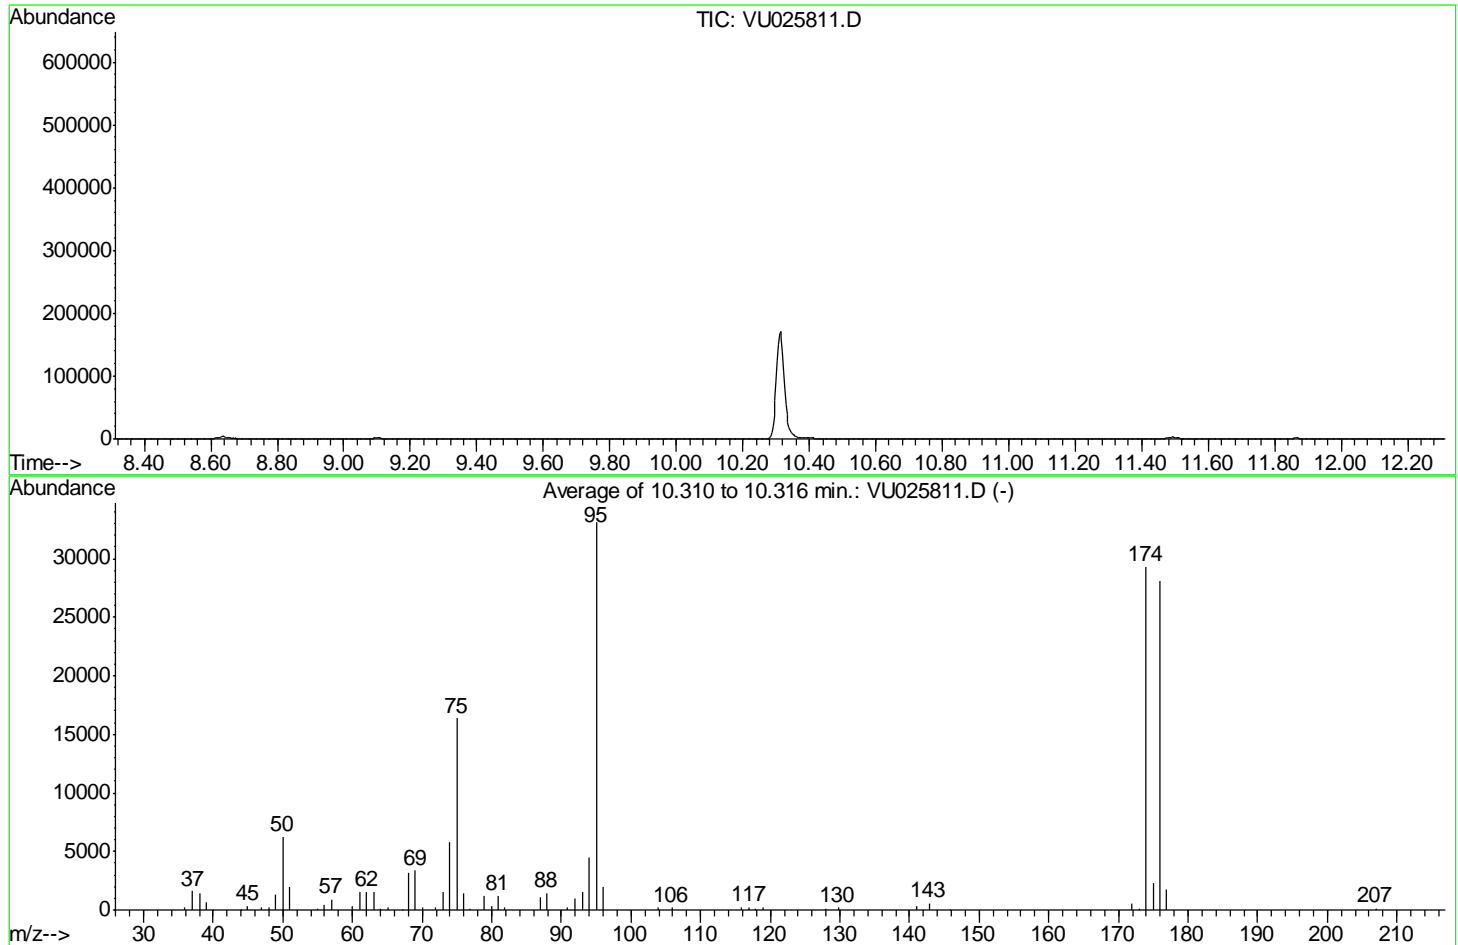

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6264	PASS
75	95	30	60	49.5	16374	PASS
95	95	100	100	100.0	33098	PASS
96	95	5	9	5.8	1916	PASS
173	174	0.00	2	0.3	102	PASS
174	95	50	100	88.6	29336	PASS
175	174	5	9	7.8	2293	PASS
176	174	95	101	95.7	28085	PASS
177	176	5	9	6.3	1760	PASS