


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080319\
 Data File : VU033579.D
 Acq On : 03 Aug 2019 09:06
 Operator : JC/SP
 Sample : BFB46
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM080319WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 05 17:10:43 2019

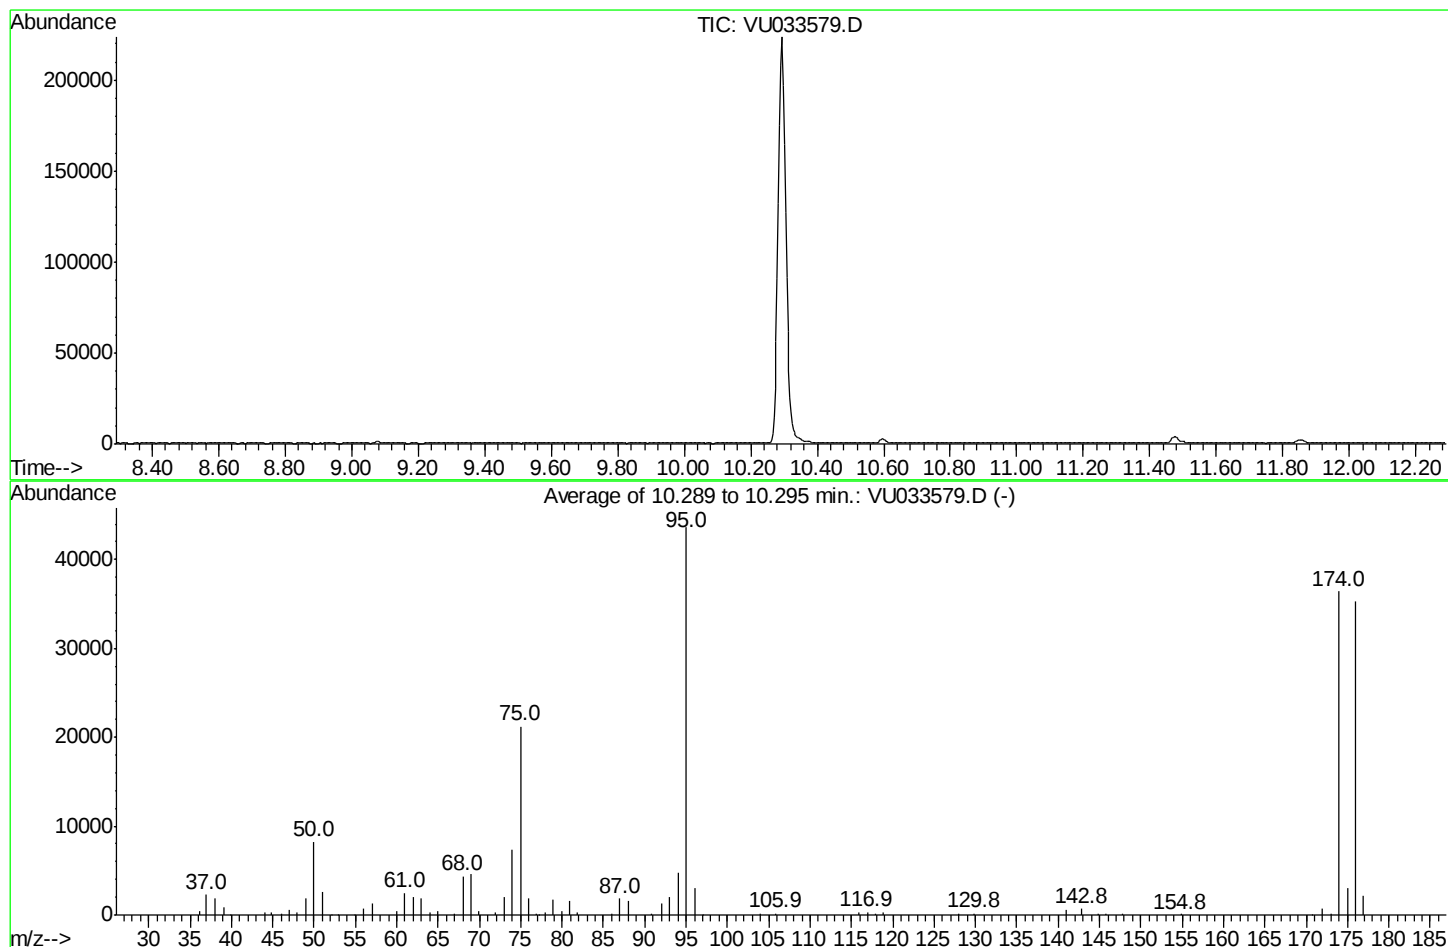

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8253	PASS
75	95	30	80	48.7	21226	PASS
95	95	100	100	100.0	43624	PASS
96	95	5	9	6.8	2961	PASS
173	174	0.00	2	0.6	206	PASS
174	95	50	120	83.5	36413	PASS
175	174	5	9	8.4	3052	PASS
176	174	95	101	97.0	35328	PASS
177	176	5	9	6.2	2186	PASS

Scan 2850 (10.254 min): VU033579.D
BFB46

m/z	Abundance
39.90	189.0
44.10	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.10	368.0
37.00	2195.0
38.00	1934.0
39.00	856.0
40.00	224.0
44.00	579.0
44.90	401.0
46.00	138.0
47.00	491.0
47.90	333.0
49.00	1762.0
50.00	8076.0
51.00	2537.0
52.10	104.0
55.00	120.0
56.00	775.0
57.00	1255.0
60.00	327.0
61.00	2468.0
62.00	1958.0
63.00	1788.0
64.10	374.0
65.00	451.0
66.90	107.0
68.00	4305.0
69.00	4446.0
69.90	457.0
71.90	266.0
73.00	1879.0
74.00	7239.0
75.00	20568.0
76.00	1947.0
76.90	218.0
78.00	191.0
78.90	1667.0
79.90	378.0
80.90	1541.0
81.90	272.0
87.00	1698.0
88.00	1611.0
90.90	169.0
92.00	1303.0
93.00	1825.0
94.00	4658.0
95.00	41632.0
96.10	3035.0
104.00	231.0
105.90	194.0
115.90	221.0
117.00	346.0
117.90	151.0
118.90	242.0
128.00	181.0
129.90	133.0
140.90	493.0
142.90	635.0
144.90	183.0
147.80	158.0
154.90	100.0
171.90	699.0
173.00	618.0
174.00	33960.0
175.00	3015.0
176.00	33488.0
176.90	2153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.10	380.0
37.00	2376.0
38.00	2035.0
39.10	896.0
39.90	237.0
44.00	621.0
44.90	384.0
46.00	117.0
47.00	558.0
48.00	337.0
49.00	1901.0
50.00	8622.0
51.00	2652.0
52.10	107.0
52.90	102.0
54.80	101.0
56.00	794.0
57.00	1279.0
59.90	396.0
61.00	2590.0
62.00	2162.0
63.00	1949.0
64.00	365.0
65.00	518.0
66.90	121.0
68.00	4485.0
69.00	4763.0
69.90	473.0
71.90	305.0
73.00	2108.0
74.00	7675.0
75.00	21880.0
76.00	2016.0
76.80	197.0
78.00	240.0
78.90	1804.0
80.00	392.0
80.90	1585.0
81.90	280.0
86.00	133.0
87.00	1915.0
88.00	1657.0
90.90	239.0
92.00	1314.0
93.00	2030.0
94.00	4946.0
95.00	44864.0
96.10	3001.0
104.00	202.0
105.90	235.0
115.90	253.0
116.90	372.0
117.90	192.0
118.90	248.0
127.90	136.0
129.80	171.0
140.90	544.0
142.90	674.0
144.90	165.0
145.80	104.0
147.80	157.0
154.80	114.0
170.70	102.0
171.90	779.0
174.00	37464.0
174.90	3240.0
176.00	36344.0
176.90	2268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.10	353.0
37.00	2250.0
38.00	1853.0
39.10	860.0
39.90	228.0
44.00	640.0
44.90	292.0
46.90	550.0
48.00	318.0
49.00	1823.0
50.00	8063.0
51.00	2668.0
56.00	792.0
57.00	1185.0
59.90	429.0
61.00	2413.0
62.00	2114.0
63.00	1890.0
64.00	334.0
65.00	524.0
66.90	128.0
68.00	4348.0
69.00	4559.0
70.00	359.0
71.90	296.0
73.00	2090.0
74.00	7297.0
75.00	21232.0
76.00	1861.0
76.80	170.0
77.20	174.0
78.00	259.0
78.90	1719.0
80.00	403.0
80.90	1530.0
81.90	309.0
86.00	169.0
86.90	1852.0
88.00	1610.0
90.80	225.0
92.00	1231.0
93.00	1999.0
94.00	4856.0
95.00	44376.0
96.00	2847.0
97.00	116.0
103.90	166.0
105.90	222.0
115.90	234.0
116.80	371.0
117.90	192.0
118.90	258.0
127.90	108.0
129.80	172.0
140.90	501.0
142.80	673.0
144.90	143.0
145.80	133.0
147.80	143.0
154.90	111.0
170.80	131.0
171.90	783.0
174.00	37816.0
175.00	2903.0
176.00	36152.0
177.00	2137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46