

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080322\
 Data File : VU050054.D
 Acq On : 03 Aug 2022 15:24
 Operator : SY/MD
 Sample : N4027-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJH0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	52	rBV2	5309	5399	1.64%	0.217%
2	1.594	68	79	94	rBV2	43754	64518	19.62%	2.596%
3	1.684	101	107	115	rBV	3854	4888	1.49%	0.197%
4	1.909	169	177	190	rVB	34187	43505	13.23%	1.750%
5	2.565	369	381	395	rVB	60809	97457	29.64%	3.921%
6	2.639	395	404	415	rBV2	4274	8786	2.67%	0.353%
7	3.890	772	793	794	rBV	2575	5413	1.65%	0.218%
8	4.636	1009	1025	1048	rBV	49238	137630	41.85%	5.537%
9	4.819	1071	1082	1096	rVB3	4724	10173	3.09%	0.409%
10	5.063	1143	1158	1181	rBV	58633	128996	39.23%	5.190%
11	5.726	1343	1364	1391	rBV2	116297	298441	90.75%	12.007%
12	6.250	1512	1527	1548	rBV	96329	186125	56.60%	7.489%
13	6.694	1651	1665	1684	rBV	73173	143035	43.50%	5.755%
14	7.568	1924	1937	1951	rBV2	31878	57697	17.54%	2.321%
15	7.899	2027	2040	2054	rBV	125125	217842	66.24%	8.765%
16	8.182	2117	2128	2141	rBV	19638	33424	10.16%	1.345%
17	8.639	2257	2270	2305	rBV4	129837	328852	100.00%	13.231%
18	8.790	2308	2317	2332	rVB3	10460	19060	5.80%	0.767%
19	9.420	2501	2513	2536	rBV	139847	235220	71.53%	9.464%
20	10.758	2914	2929	2943	rBV2	60879	96829	29.44%	3.896%
21	11.690	3213	3219	3227	rBV5	2698	3657	1.11%	0.147%
22	11.812	3245	3257	3277	rBV	115458	184857	56.21%	7.438%
23	12.195	3365	3376	3390	rBV	105411	167818	51.03%	6.752%
24	12.893	3585	3593	3602	rBV5	4139	5848	1.78%	0.235%


Sum of corrected areas: 2485470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080322\
Data File : VU050054.D
Acq On : 03 Aug 2022 15:24
Operator : SY/MD
Sample : N4027-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

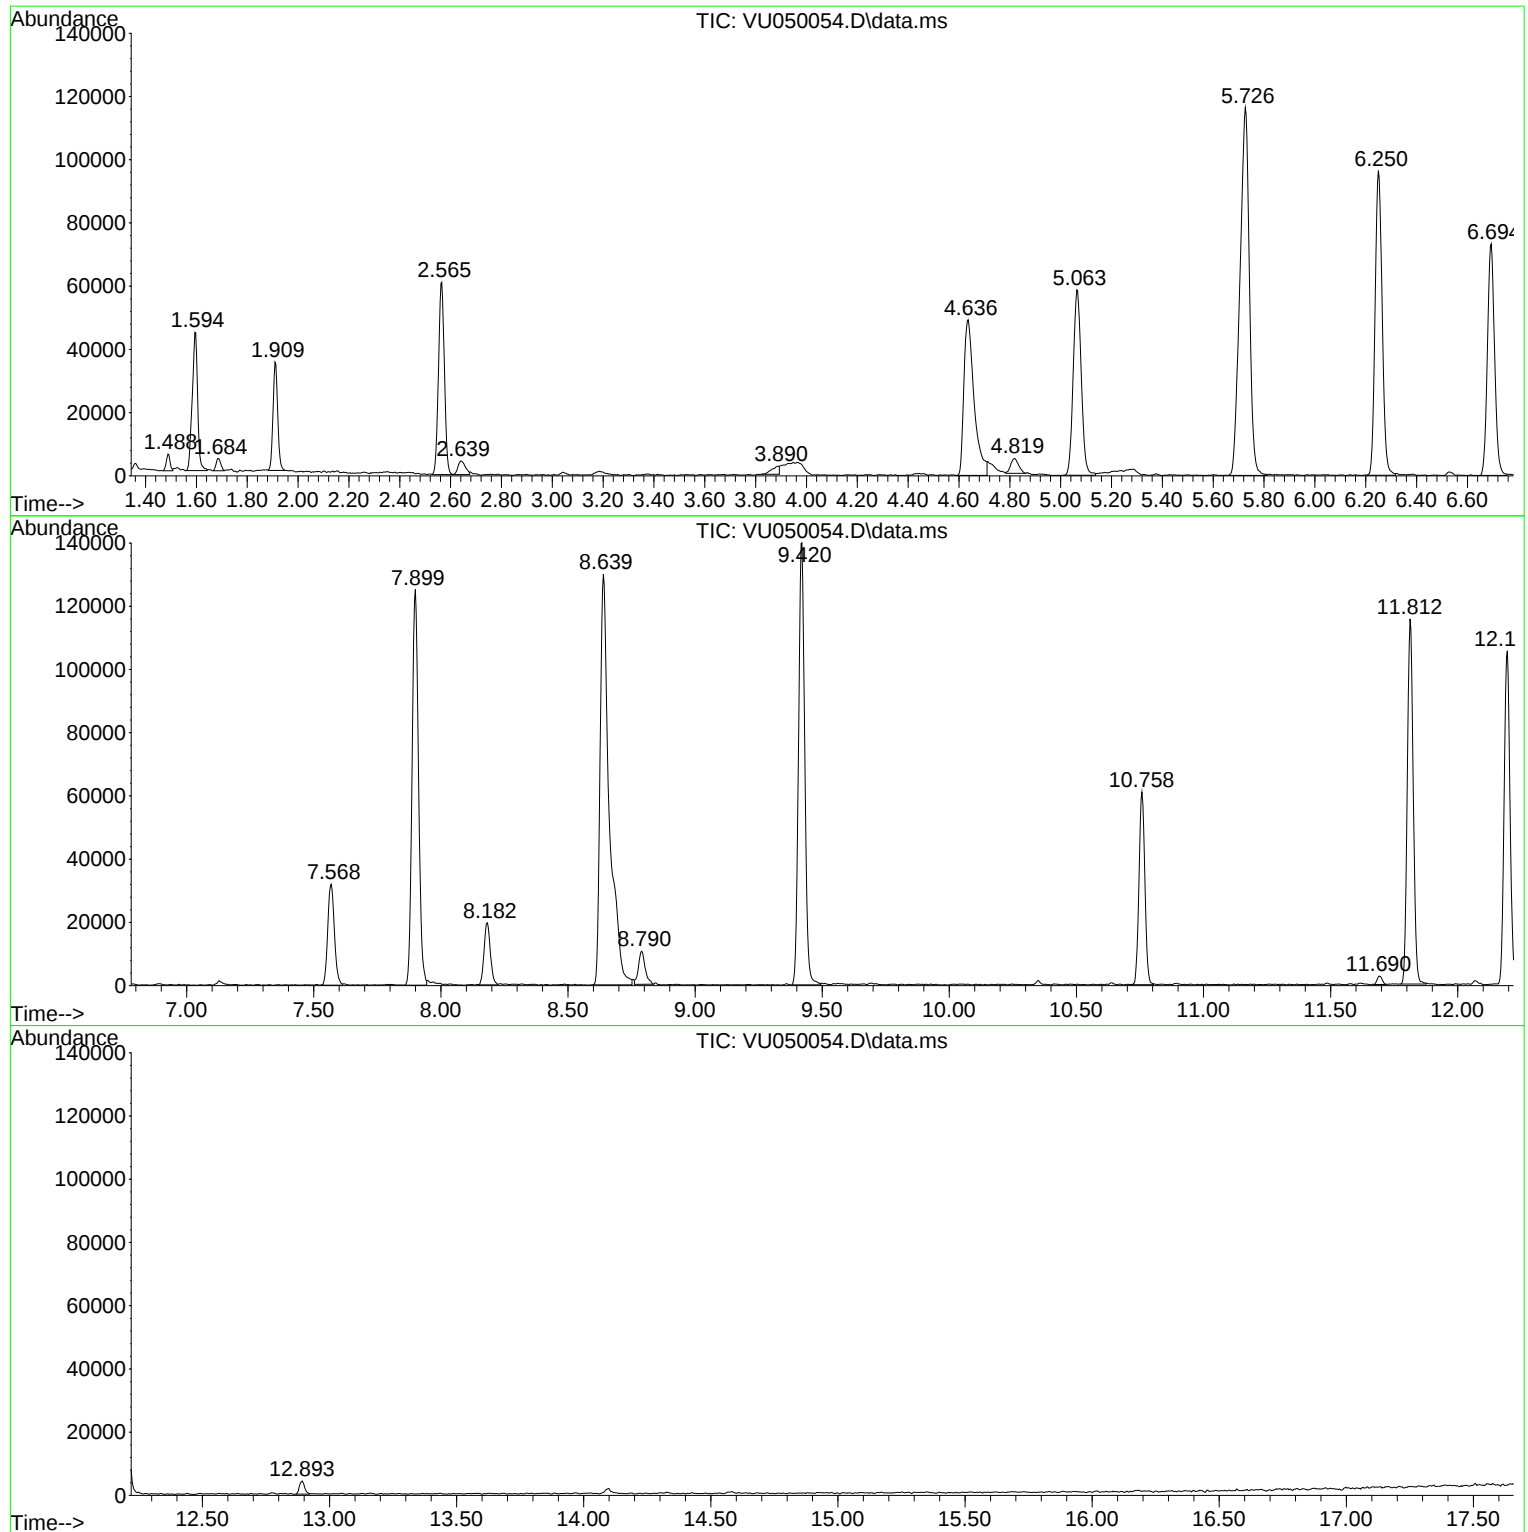

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080322\
Data File : VU050054.D
Acq On : 03 Aug 2022 15:24
Operator : SY/MD
Sample : N4027-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080322\
Data File : VU050054.D
Acq On : 03 Aug 2022 15:24
Operator : SY/MD
Sample : N4027-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc