
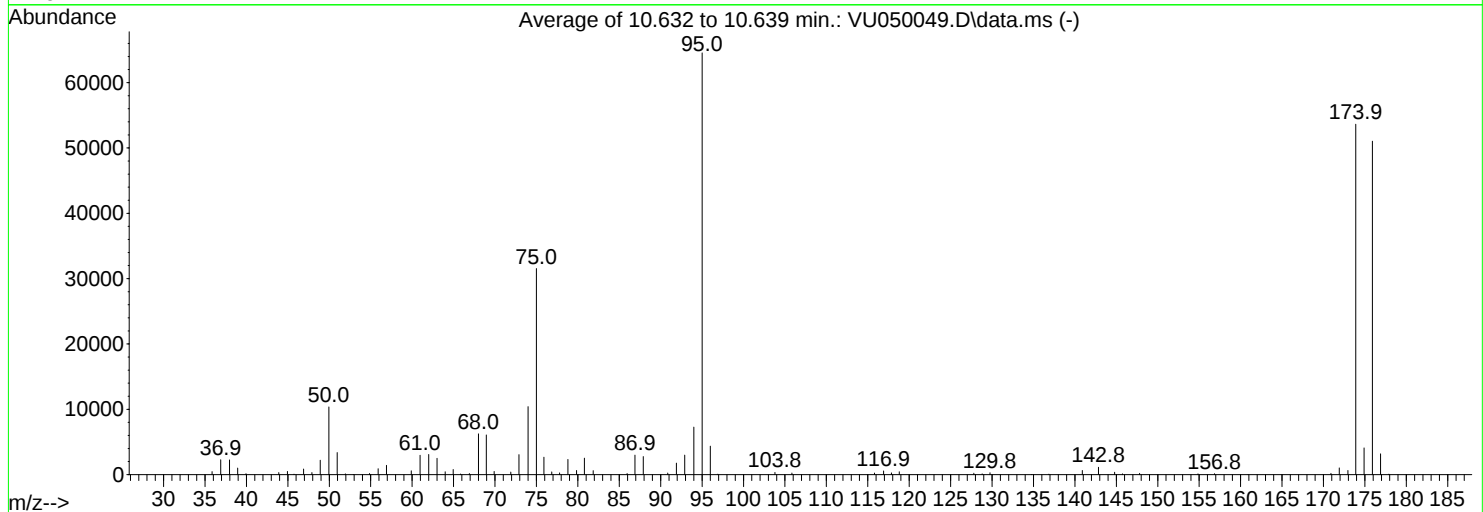


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080322\
 Data File : VU050049.D
 Acq On : 03 Aug 2022 11:32
 Operator : SY/MD
 Sample : BFB099
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB099

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Aug 04 01:44:33 2022

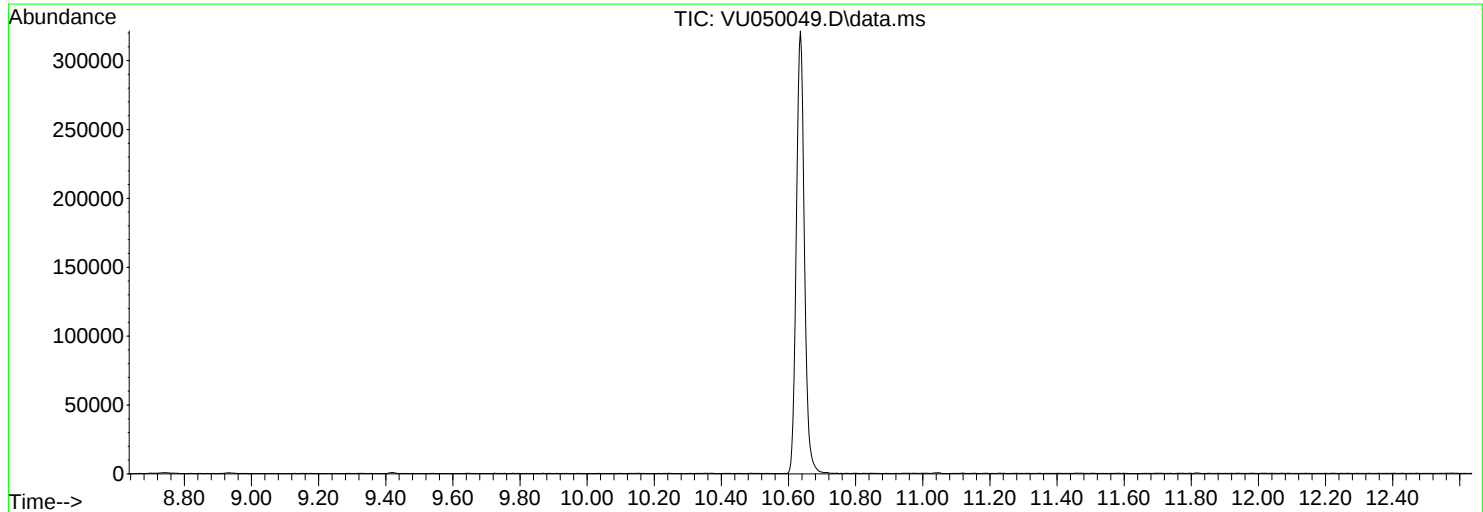

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10375	PASS
75	95	30	80	48.9	31541	PASS
95	95	100	100	100.0	64560	PASS
96	95	5	9	6.8	4358	PASS
173	174	0.00	2	1.2	631	PASS
174	95	50	120	83.1	53637	PASS
175	174	5	9	7.6	4098	PASS
176	174	95	101	95.1	51035	PASS
177	176	5	9	6.2	3177	PASS

m/z	Abundance
43.90	313.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	453.0
36.90	2350.0
37.90	2307.0
38.90	1017.0
40.00	152.0
43.90	674.0
44.90	541.0
46.90	862.0
47.90	344.0
48.90	2261.0
49.90	10651.0
51.00	3500.0
52.00	120.0
52.90	109.0
54.90	188.0
55.90	946.0
56.90	1421.0
59.90	602.0
61.00	3068.0
62.00	3208.0
63.00	2622.0
64.00	445.0
65.00	773.0
65.90	119.0
66.90	186.0
68.00	6195.0
69.00	6071.0
69.90	514.0
71.90	339.0
72.90	2996.0
74.00	10670.0
75.00	31688.0
75.90	2844.0
76.80	405.0
77.90	308.0
78.80	2317.0
79.80	638.0
80.80	2507.0
81.80	639.0
85.90	133.0
86.90	2966.0
87.90	2741.0
90.90	255.0
91.90	1664.0
92.90	2933.0
94.00	7116.0
95.00	64352.0
96.00	4381.0
103.80	344.0
105.90	238.0
115.80	226.0
116.90	550.0
117.80	252.0
118.80	452.0
127.80	239.0
128.80	101.0
129.70	289.0
136.80	105.0
140.90	651.0
142.80	1007.0
144.80	420.0
145.80	135.0
147.80	173.0
154.80	133.0
156.90	142.0
170.90	190.0
171.90	970.0
172.90	641.0
173.90	52648.0
174.90	4055.0
175.90	49936.0
176.90	3279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	485.0
36.90	2383.0
38.00	2346.0
39.00	1012.0
40.00	151.0
43.90	644.0
44.90	497.0
45.80	106.0
46.90	900.0
47.90	335.0
48.90	2296.0
50.00	10705.0
51.00	3521.0
51.90	134.0
54.90	169.0
55.90	942.0
56.90	1471.0
59.90	624.0
61.00	3052.0
62.00	3163.0
63.00	2540.0
64.00	460.0
64.90	797.0
65.90	105.0
66.90	181.0
68.00	6385.0
69.00	6221.0
69.90	509.0
71.90	411.0
72.90	3216.0
74.00	10697.0
75.00	32552.0
75.90	2754.0
76.90	433.0
77.80	280.0
78.80	2378.0
79.90	654.0
80.80	2603.0
81.80	634.0
85.90	192.0
86.90	3093.0
87.90	2866.0
90.90	249.0
91.90	1806.0
92.90	3106.0
94.00	7477.0
95.00	66352.0
96.00	4494.0
96.90	118.0
103.80	348.0
105.80	245.0
115.80	249.0
116.90	604.0
117.90	282.0
118.80	449.0
127.80	227.0
128.80	127.0
129.80	294.0
136.90	106.0
140.90	651.0
142.90	1146.0
144.80	367.0
145.80	131.0
147.80	212.0
154.80	136.0
156.90	137.0
160.90	110.0
170.90	203.0
171.90	1079.0
173.00	635.0
173.90	55152.0
174.90	4201.0
175.90	52464.0
176.90	3271.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.80	461.0
36.90	2106.0
38.00	2149.0
39.00	966.0
39.90	153.0
43.90	591.0
45.00	428.0
45.70	100.0
46.90	808.0
47.90	303.0
48.90	2089.0
50.00	9768.0
50.90	3134.0
51.90	148.0
54.80	155.0
55.90	815.0
56.90	1408.0
59.90	572.0
60.90	2787.0
62.00	2903.0
63.00	2347.0
64.00	430.0
64.90	821.0
65.80	101.0
66.90	158.0
68.00	6145.0
68.90	5913.0
69.90	462.0
71.90	426.0
72.90	3002.0
74.00	9855.0
75.00	30384.0
75.90	2413.0
76.90	424.0
77.70	234.0
78.80	2268.0
79.90	611.0
80.80	2489.0
81.90	569.0
86.00	191.0
86.90	2942.0
87.90	2678.0
90.80	231.0
91.90	1838.0
92.90	2938.0
94.00	7249.0
95.00	62976.0
96.00	4198.0
96.90	130.0
103.80	367.0
105.80	242.0
115.80	261.0
116.90	575.0
117.90	285.0
118.80	397.0
127.80	206.0
128.80	130.0
129.80	277.0
134.80	105.0
140.90	622.0
142.90	1216.0
144.80	318.0
145.70	122.0
147.80	211.0
154.90	123.0
156.80	133.0
170.90	185.0
171.90	1068.0
173.00	618.0
173.90	53112.0
174.90	4037.0
175.90	50704.0
176.90	2981.0
177.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099