

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
 Data File : VU025831.D
 Acq On : 03 Aug 2018 20:21
 Operator : MD/SY
 Sample : J4340-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E5F71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.754	49	51	52	rBV	45	21	0.00%	0.000%
2	0.761	52	53	54	rVB	128	25	0.00%	0.000%
3	0.777	54	58	59	rBV2	191	132	0.00%	0.001%
4	0.809	63	68	72	rBV2	439	389	0.01%	0.002%
5	0.835	72	76	77	rBV2	372	261	0.00%	0.001%
6	0.909	95	99	105	rVB2	416	535	0.01%	0.003%
7	0.934	105	107	108	rBV2	178	88	0.00%	0.000%
8	1.089	137	155	172	rBV	416772	460828	7.19%	2.350%
9	1.401	245	252	266	rBV	132680	141505	2.21%	0.721%
10	1.680	332	339	355	rVB	96553	123688	1.93%	0.631%
11	2.272	513	523	536	rBV	222182	333211	5.20%	1.699%
12	2.616	626	630	636	rBV3	741	883	0.01%	0.005%
13	2.835	692	698	710	rVB5	1732	2798	0.04%	0.014%
14	2.986	736	745	757	rVB3	6957	12542	0.20%	0.064%
15	3.249	821	827	829	rBV2	403	383	0.01%	0.002%
16	3.275	832	835	838	rVB	306	164	0.00%	0.001%
17	3.294	838	841	844	rBV	221	163	0.00%	0.001%
18	3.330	850	852	856	rBV2	330	237	0.00%	0.001%
19	3.349	857	858	859	rBV2	151	47	0.00%	0.000%
20	3.442	885	887	891	rVB2	378	200	0.00%	0.001%
21	3.487	897	901	903	rBV	284	287	0.00%	0.001%
22	3.542	915	918	921	rBV	376	264	0.00%	0.001%
23	3.587	929	932	935	rBV2	261	176	0.00%	0.001%
24	3.626	941	944	945	rBV	306	128	0.00%	0.001%
25	3.664	952	956	960	rBV3	379	278	0.00%	0.001%
26	3.700	963	967	970	rVB2	534	374	0.01%	0.002%
27	3.719	970	973	974	rBV	151	81	0.00%	0.000%
28	3.729	974	976	979	rBV	221	137	0.00%	0.001%
29	3.777	989	991	995	rVB	289	158	0.00%	0.001%
30	3.796	995	997	998	rBV	132	73	0.00%	0.000%
31	3.915	1032	1034	1036	rBV2	136	73	0.00%	0.000%
32	3.979	1050	1054	1055	rBV2	461	238	0.00%	0.001%
33	4.063	1077	1080	1085	rBV2	451	394	0.01%	0.002%
34	4.092	1086	1089	1091	rBV2	317	203	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
 Data File : VU025831.D
 Acq On : 03 Aug 2018 20:21
 Operator : MD/SY
 Sample : J4340-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E5F71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	4.230	1101	1132	1164	rBV2	1224102	3187692	49.75%	16.253%
36	4.651	1246	1263	1287	rBV	186672	433453	6.76%	2.210%
37	4.777	1300	1302	1304	rVB2	492	205	0.00%	0.001%
38	4.799	1307	1309	1311	rBV2	313	179	0.00%	0.001%
39	4.883	1330	1335	1339	rBV3	1045	1115	0.02%	0.006%
40	4.950	1355	1356	1359	rBV	234	77	0.00%	0.000%
41	4.995	1366	1370	1376	rBV4	854	840	0.01%	0.004%
42	5.063	1388	1391	1392	rBV2	409	204	0.00%	0.001%
43	5.217	1433	1439	1447	rBV2	296	485	0.01%	0.002%
44	5.346	1455	1479	1509	rBV2	360504	1069632	16.69%	5.454%
45	5.539	1530	1539	1541	rBV4	2868	4263	0.07%	0.022%
46	5.680	1579	1583	1585	rBV2	580	469	0.01%	0.002%
47	5.764	1606	1609	1613	rBV2	395	304	0.00%	0.002%
48	5.818	1624	1626	1628	rVB2	375	192	0.00%	0.001%
49	5.889	1628	1648	1673	rBV	389798	763863	11.92%	3.895%
50	6.188	1726	1741	1767	rBV	594954	1143665	17.85%	5.831%
51	6.333	1773	1786	1808	rVB	241563	479933	7.49%	2.447%
52	6.455	1820	1824	1828	rBV5	989	859	0.01%	0.004%
53	6.487	1832	1834	1837	rVB2	362	193	0.00%	0.001%
54	6.507	1837	1840	1843	rBV2	347	274	0.00%	0.001%
55	6.535	1847	1849	1853	rBV2	308	316	0.00%	0.002%
56	6.648	1883	1884	1889	rVB2	279	167	0.00%	0.001%
57	6.828	1935	1940	1942	rBV3	584	465	0.01%	0.002%
58	6.857	1943	1949	1954	rVB4	877	1019	0.02%	0.005%
59	6.876	1954	1955	1958	rBV2	373	191	0.00%	0.001%
60	7.047	2001	2008	2010	rBV3	1652	1649	0.03%	0.008%
61	7.134	2030	2035	2037	rBV2	374	365	0.01%	0.002%
62	7.230	2053	2065	2085	rBV	139581	248065	3.87%	1.265%
63	7.507	2145	2151	2154	rBV3	397	505	0.01%	0.003%
64	7.568	2157	2170	2191	rBV	486501	861265	13.44%	4.391%
65	7.854	2247	2259	2279	rBV	99870	171543	2.68%	0.875%
66	8.159	2352	2354	2357	rBV2	627	340	0.01%	0.002%
67	8.230	2361	2376	2392	rVV	3794482	6407812	100.00%	32.671%
68	8.314	2394	2402	2436	rVB	306993	552798	8.63%	2.819%
69	8.706	2522	2524	2527	rBV2	317	149	0.00%	0.001%
70	8.896	2580	2583	2585	rBV	305	172	0.00%	0.001%
71	8.979	2607	2609	2613	rBV2	330	134	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
 Data File : VU025831.D
 Acq On : 03 Aug 2018 20:21
 Operator : MD/SY
 Sample : J4340-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E5F71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	9.034	2624	2626	2630	rBV	346	253	0.00%	0.001%
73	9.092	2631	2644	2686	rVB	560326	941126	14.69%	4.798%
74	9.256	2688	2695	2703	rBV3	742	1142	0.02%	0.006%
75	9.452	2754	2756	2759	rBV2	241	111	0.00%	0.001%
76	9.526	2777	2779	2781	rBV2	375	162	0.00%	0.001%
77	10.191	2982	2986	2988	rBV	276	248	0.00%	0.001%
78	10.268	3007	3010	3013	rVB2	412	256	0.00%	0.001%
79	10.310	3020	3023	3030	rBV4	1104	1282	0.02%	0.007%
80	10.436	3050	3062	3080	rBV	330484	535322	8.35%	2.729%
81	10.664	3131	3133	3134	rBV2	310	156	0.00%	0.001%
82	10.982	3230	3232	3235	rBV	329	209	0.00%	0.001%
83	11.082	3261	3263	3265	rBV2	398	223	0.00%	0.001%
84	11.236	3308	3311	3312	rBV	409	268	0.00%	0.001%
85	11.313	3332	3335	3338	rBV	342	248	0.00%	0.001%
86	11.487	3376	3389	3405	rBV	560039	891376	13.91%	4.545%
87	11.863	3493	3506	3527	rBV	508435	824263	12.86%	4.203%
88	12.307	3639	3644	3647	rBV4	567	675	0.01%	0.003%


Sum of corrected areas: 19613136

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080418\
Data File : VU025831.D
Acq On : 03 Aug 2018 20:21
Operator : MD/SY
Sample : J4340-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

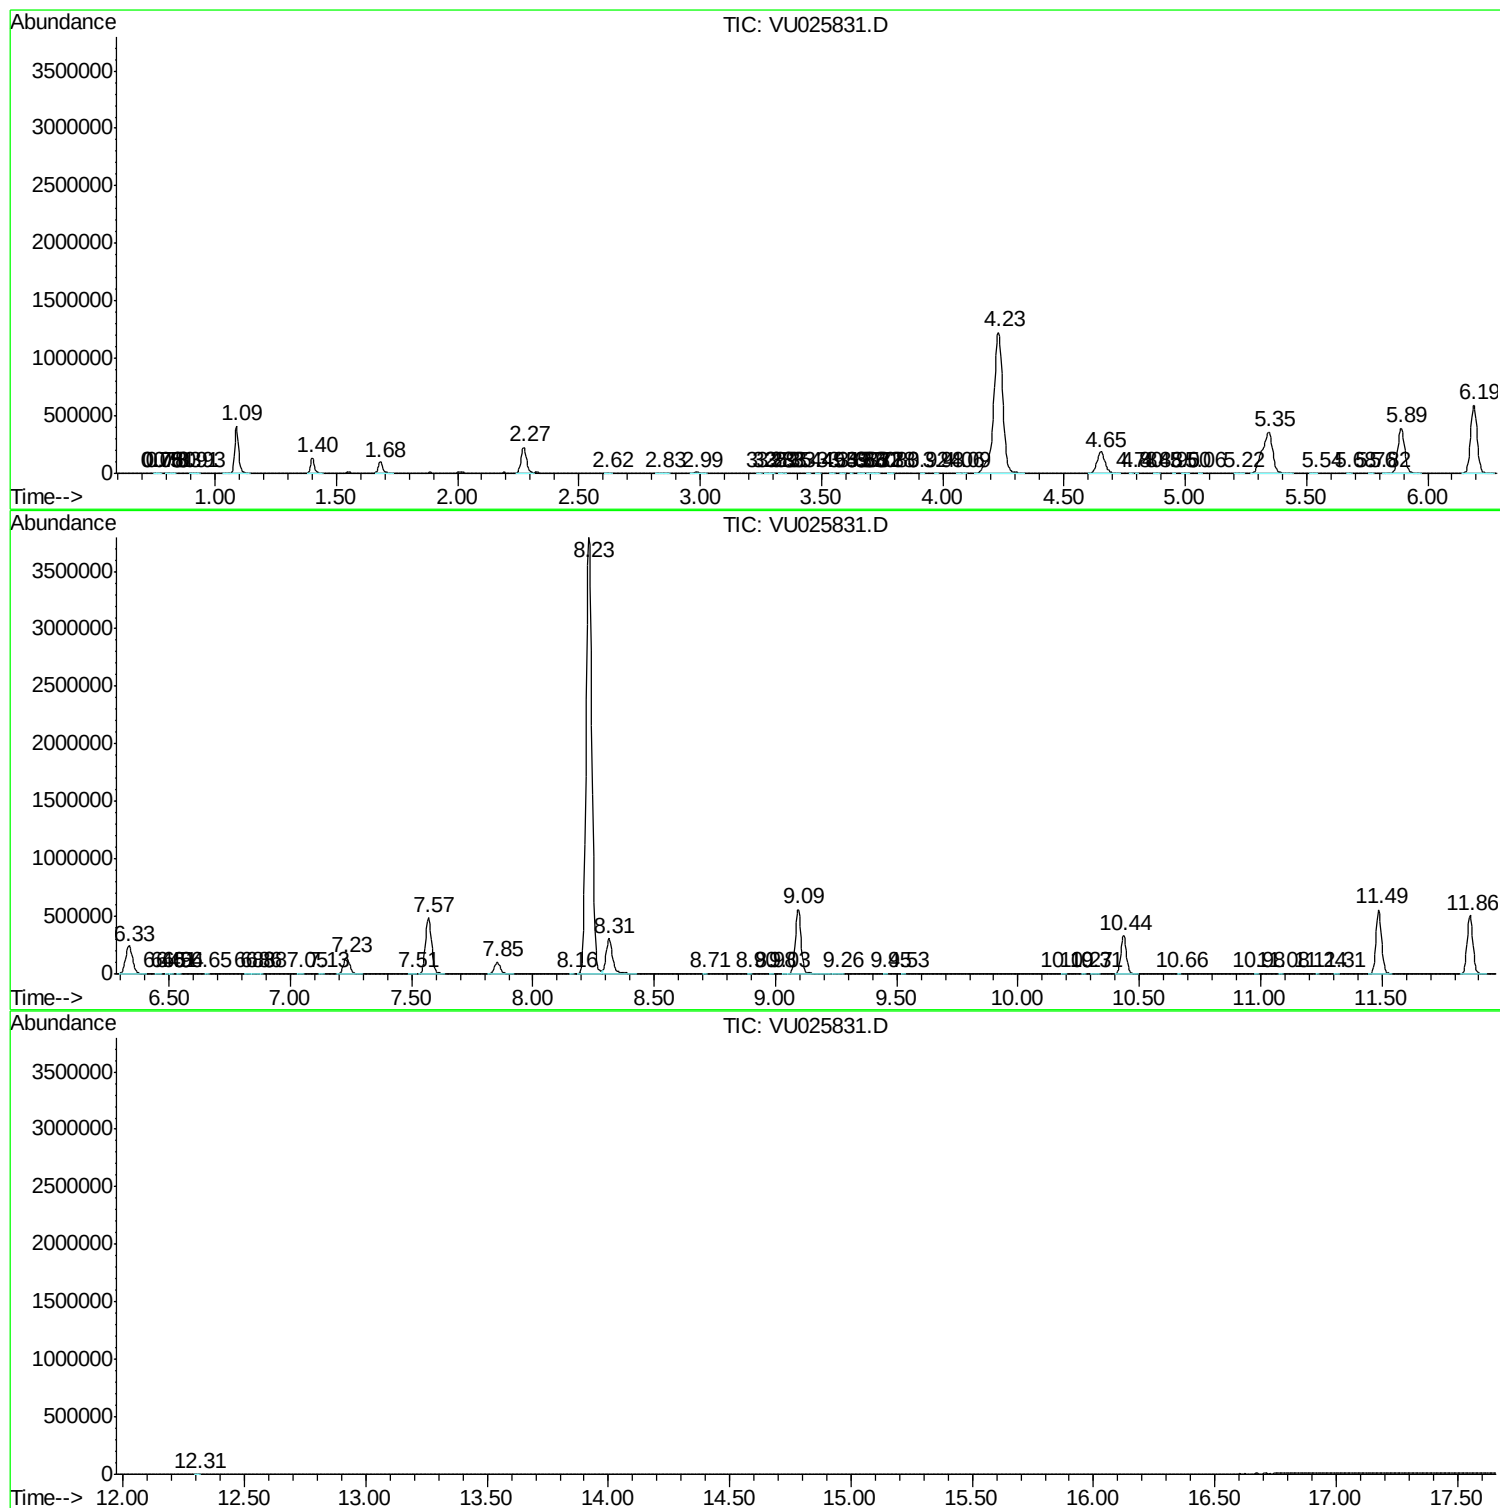

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080418\
Data File : VU025831.D
Acq On : 03 Aug 2018 20:21
Operator : MD/SY
Sample : J4340-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080418\
Data File : VU025831.D
Acq On : 03 Aug 2018 20:21
Operator : MD/SY
Sample : J4340-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc