

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
 Data File : VU025832.D
 Acq On : 03 Aug 2018 20:44
 Operator : MD/SY
 Sample : J4340-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E5F72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.642	15	16	17	rBV	119	37	0.00%	0.000%
2	0.658	17	21	22	rVV2	149	90	0.00%	0.000%
3	0.809	65	68	70	rBV2	423	309	0.00%	0.002%
4	0.876	86	89	91	rBV	267	169	0.00%	0.001%
5	1.005	126	129	131	rBV2	298	240	0.00%	0.001%
6	1.047	136	142	143	rBV	464	417	0.01%	0.002%
7	1.089	147	155	176	rVV	418826	458948	7.02%	2.324%
8	1.400	245	252	263	rBV	131521	139409	2.13%	0.706%
9	1.683	332	340	355	rVB	100174	123401	1.89%	0.625%
10	2.272	514	523	534	rVB	229832	342216	5.24%	1.733%
11	2.934	727	729	734	rBV2	448	383	0.01%	0.002%
12	2.989	735	746	757	rVB2	7334	13845	0.21%	0.070%
13	3.037	757	761	765	rBV3	410	330	0.01%	0.002%
14	3.153	794	797	802	rVB2	269	174	0.00%	0.001%
15	3.195	808	810	812	rBV2	140	70	0.00%	0.000%
16	3.243	822	825	829	rBV2	428	375	0.01%	0.002%
17	3.285	835	838	839	rBV	223	145	0.00%	0.001%
18	3.339	851	855	859	rBV2	326	371	0.01%	0.002%
19	3.375	864	866	867	rBV2	232	88	0.00%	0.000%
20	3.561	921	924	925	rBV2	328	222	0.00%	0.001%
21	3.616	937	941	943	rBV2	280	253	0.00%	0.001%
22	3.706	964	969	972	rBV	500	474	0.01%	0.002%
23	3.847	1010	1013	1016	rVB2	191	120	0.00%	0.001%
24	3.886	1023	1025	1027	rBV2	176	116	0.00%	0.001%
25	3.902	1027	1030	1032	rBV2	260	171	0.00%	0.001%
26	3.941	1038	1042	1047	rBV3	323	375	0.01%	0.002%
27	3.966	1047	1050	1054	rVB2	219	186	0.00%	0.001%
28	3.998	1054	1060	1066	rBV2	1088	1278	0.02%	0.006%
29	4.114	1093	1096	1098	rBV2	297	193	0.00%	0.001%
30	4.124	1098	1099	1100	rVB2	120	23	0.00%	0.000%
31	4.230	1102	1132	1164	rBV2	1222864	3180783	48.68%	16.109%
32	4.651	1247	1263	1284	rBV	183033	430456	6.59%	2.180%
33	4.957	1355	1358	1359	rBV	327	202	0.00%	0.001%
34	5.031	1376	1381	1385	rVB2	354	362	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
 Data File : VU025832.D
 Acq On : 03 Aug 2018 20:44
 Operator : MD/SY
 Sample : J4340-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E5F72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	5.072	1387	1394	1395	rBV4	694	571	0.01%	0.003%
36	5.127	1409	1411	1412	rBV	146	79	0.00%	0.000%
37	5.156	1418	1420	1422	rVB	271	105	0.00%	0.001%
38	5.172	1422	1425	1426	rBV2	332	225	0.00%	0.001%
39	5.214	1432	1438	1439	rBV2	312	319	0.00%	0.002%
40	5.346	1454	1479	1504	rBV2	358871	1072449	16.41%	5.431%
41	5.542	1528	1540	1554	rVB3	3994	8599	0.13%	0.044%
42	5.596	1554	1557	1561	rVB2	441	297	0.00%	0.002%
43	5.619	1561	1564	1566	rBV	261	205	0.00%	0.001%
44	5.680	1578	1583	1585	rBV2	576	522	0.01%	0.003%
45	5.712	1589	1593	1596	rVV3	249	212	0.00%	0.001%
46	5.748	1601	1604	1605	rBV	303	170	0.00%	0.001%
47	5.818	1623	1626	1631	rBV3	213	161	0.00%	0.001%
48	5.889	1634	1648	1673	rBV	388410	766686	11.73%	3.883%
49	6.191	1726	1742	1773	rBV	603287	1160809	17.77%	5.879%
50	6.336	1773	1787	1804	rVV	243821	483203	7.40%	2.447%
51	6.429	1812	1816	1819	rBV3	576	466	0.01%	0.002%
52	6.506	1838	1840	1841	rVB	274	75	0.00%	0.000%
53	6.558	1848	1856	1859	rBV3	446	588	0.01%	0.003%
54	6.625	1874	1877	1881	rVB2	281	240	0.00%	0.001%
55	6.651	1882	1885	1887	rBV2	254	85	0.00%	0.000%
56	6.667	1887	1890	1898	rBV3	230	360	0.01%	0.002%
57	6.747	1906	1915	1919	rVB4	644	757	0.01%	0.004%
58	6.770	1919	1922	1925	rBV3	302	201	0.00%	0.001%
59	6.821	1934	1938	1940	rBV	406	258	0.00%	0.001%
60	6.841	1940	1944	1945	rBV2	483	307	0.00%	0.002%
61	7.002	1991	1994	1997	rBV	227	171	0.00%	0.001%
62	7.120	2027	2031	2032	rBV	490	354	0.01%	0.002%
63	7.230	2053	2065	2092	rBV	138948	249332	3.82%	1.263%
64	7.358	2103	2105	2106	rBV	470	232	0.00%	0.001%
65	7.416	2121	2123	2124	rBV	361	135	0.00%	0.001%
66	7.490	2140	2146	2149	rBV3	413	491	0.01%	0.002%
67	7.571	2157	2171	2190	rBV	493827	860431	13.17%	4.358%
68	7.854	2247	2259	2277	rBV2	100267	169521	2.59%	0.859%
69	8.104	2334	2337	2342	rBV4	441	277	0.00%	0.001%
70	8.230	2362	2376	2393	rBV	3845885	6533980	100.00%	33.090%
71	8.313	2394	2402	2430	rVB	301459	539031	8.25%	2.730%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU080418\
Data File : VU025832.D
Acq On : 03 Aug 2018 20:44
Operator : MD/SY
Sample : J4340-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F72

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis

72	8.677	2510	2515	2516	rBV2	440	317	0.00%	0.002%
73	8.760	2538	2541	2545	rBV2	403	375	0.01%	0.002%
74	8.837	2563	2565	2566	rBV	317	134	0.00%	0.001%
75	8.892	2579	2582	2586	rBV2	594	493	0.01%	0.002%
76	9.091	2632	2644	2668	rBV	559715	935217	14.31%	4.736%
77	9.294	2705	2707	2709	rBV2	486	287	0.00%	0.001%
78	9.448	2751	2755	2757	rBV	525	392	0.01%	0.002%
79	9.503	2770	2772	2776	rBV2	329	289	0.00%	0.001%
80	9.767	2852	2854	2856	rBV2	218	101	0.00%	0.001%
81	9.786	2856	2860	2861	rBV2	738	491	0.01%	0.002%
82	10.127	2962	2966	2969	rBV3	331	307	0.00%	0.002%
83	10.214	2986	2993	2995	rBV2	548	507	0.01%	0.003%
84	10.320	3022	3026	3029	rVB3	964	776	0.01%	0.004%
85	10.435	3050	3062	3082	rVB	335404	530193	8.11%	2.685%
86	11.487	3377	3389	3406	rBV	581543	908943	13.91%	4.603%
87	11.863	3493	3506	3525	rBV	505283	818906	12.53%	4.147%


Sum of corrected areas: 19745863

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU080418\
Data File : VU025832.D
Acq On : 03 Aug 2018 20:44
Operator : MD/SY
Sample : J4340-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

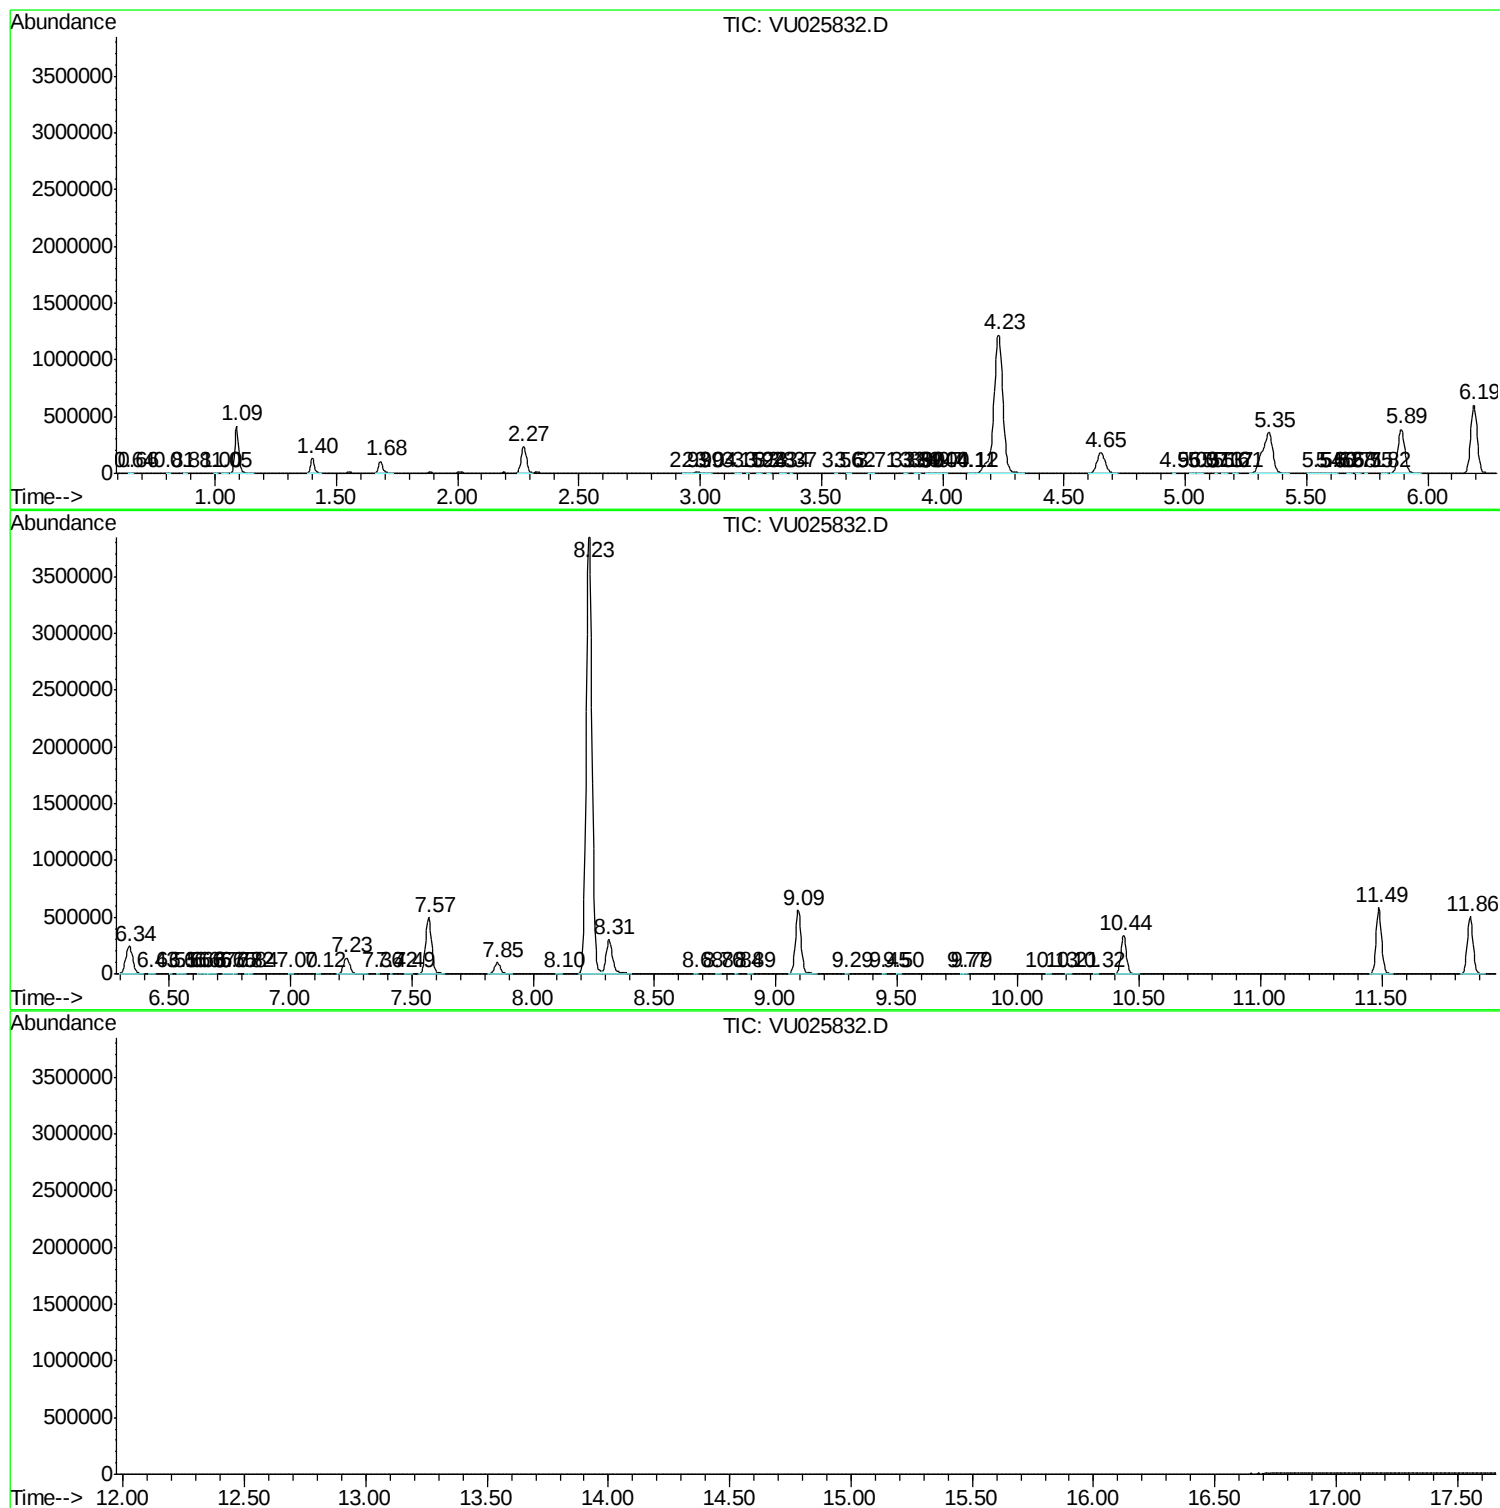

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080418\
Data File : VU025832.D
Acq On : 03 Aug 2018 20:44
Operator : MD/SY
Sample : J4340-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU080418\
Data File : VU025832.D
Acq On : 03 Aug 2018 20:44
Operator : MD/SY
Sample : J4340-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E5F72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc