


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU080418\
 Data File : VU025818.D
 Acq On : 03 Aug 2018 14:56
 Operator : MD/SY
 Sample : BFB53
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB53

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 06 01:30:36 2018

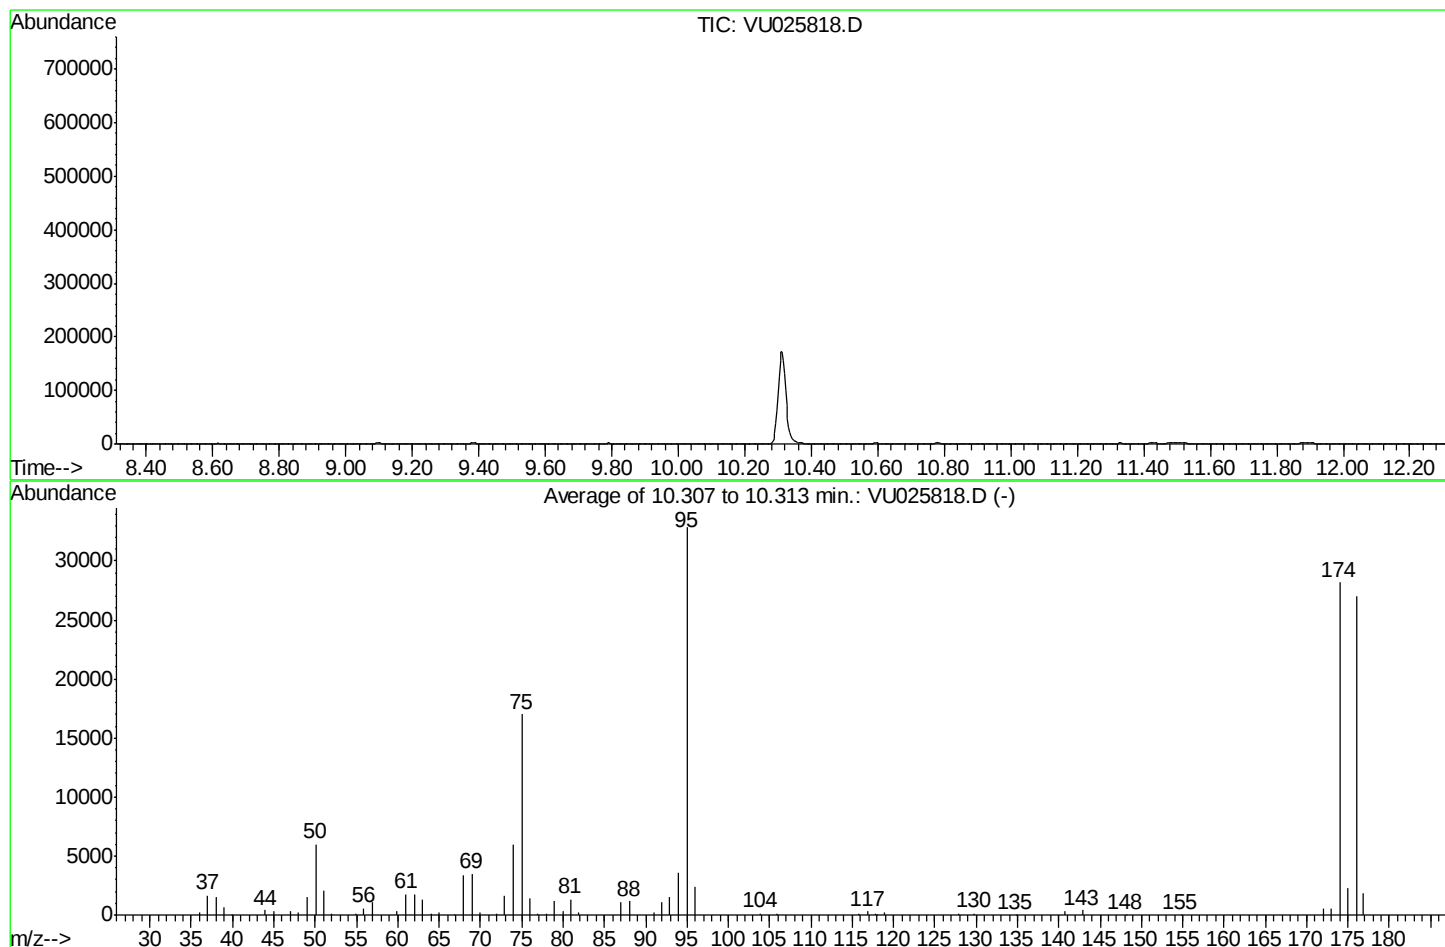

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	5988	PASS
75	95	30	80	51.7	16985	PASS
95	95	100	100	100.0	32853	PASS
96	95	5	9	7.3	2393	PASS
173	174	0.00	2	1.8	495	PASS
174	95	50	120	85.8	28197	PASS
175	174	5	9	8.0	2267	PASS
176	174	95	101	95.7	26981	PASS
177	176	5	9	6.7	1810	PASS

Scan 3011 (10.271 min): VU025818.D
BFB53

m/z	Abundance
44.10	197.0
207.20	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	289.0
37.00	1563.0
38.00	1487.0
39.00	614.0
39.90	104.0
44.00	560.0
44.90	306.0
47.00	306.0
47.90	187.0
49.00	1245.0
50.00	6092.0
51.00	2011.0
51.90	121.0
54.90	120.0
55.90	536.0
57.00	1141.0
59.90	328.0
61.00	1757.0
62.00	1639.0
63.00	1208.0
64.00	128.0
65.00	212.0
68.00	3204.0
69.00	3201.0
69.90	236.0
71.90	121.0
72.90	1544.0
74.00	5845.0
75.00	16244.0
76.00	1370.0
78.00	124.0
78.90	1189.0
80.00	355.0
80.90	1333.0
81.90	225.0
87.00	970.0
88.00	1073.0
91.00	227.0
92.00	998.0
92.90	1419.0
94.00	3408.0
95.00	30608.0
96.00	2477.0
103.90	162.0
106.00	122.0
115.80	142.0
116.90	285.0
117.80	108.0
118.80	235.0
127.90	179.0
129.80	161.0
140.80	345.0
142.80	351.0
148.10	132.0
172.00	500.0
173.00	412.0
174.00	26200.0
174.90	2140.0
176.00	24656.0
176.90	1672.0
207.00	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
36.00	273.0
37.00	1694.0
38.00	1598.0
39.00	652.0
44.00	623.0
45.00	390.0
47.00	370.0
48.00	170.0
49.00	1545.0
50.00	6114.0
51.00	2221.0
51.90	101.0
54.90	134.0
55.90	597.0
57.00	1141.0
59.90	328.0
61.00	1866.0
62.00	1806.0
63.00	1423.0
64.00	169.0
64.90	218.0
68.00	3510.0
69.00	3633.0
69.90	254.0
71.90	136.0
73.00	1743.0
74.00	6195.0
75.00	17488.0
76.00	1440.0
77.00	109.0
78.00	133.0
78.90	1265.0
80.00	394.0
80.90	1365.0
81.90	275.0
87.00	1156.0
88.00	1188.0
90.90	234.0
92.00	1046.0
92.90	1590.0
94.00	3670.0
95.00	34032.0
96.00	2457.0
103.90	171.0
106.00	125.0
115.80	150.0
116.90	342.0
117.70	107.0
118.90	256.0
127.90	158.0
129.80	160.0
140.80	383.0
142.80	430.0
171.90	533.0
173.00	532.0
174.00	28976.0
174.90	2317.0
176.00	27752.0
176.90	1886.0
207.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53

m/z	Abundance
35.90	239.0
37.00	1709.0
38.00	1519.0
39.00	658.0
43.90	705.0
45.00	422.0
47.00	380.0
48.00	195.0
49.00	1642.0
50.10	5760.0
51.00	2125.0
54.90	138.0
55.90	565.0
56.90	1015.0
59.90	308.0
61.00	1675.0
62.00	1771.0
63.00	1407.0
64.00	183.0
64.90	244.0
66.90	109.0
68.00	3450.0
69.00	3645.0
69.90	228.0
72.00	151.0
73.00	1749.0
74.00	5989.0
75.00	17224.0
76.00	1466.0
76.90	127.0
78.00	110.0
78.90	1188.0
79.90	372.0
80.90	1317.0
81.90	262.0
87.00	1231.0
88.00	1273.0
90.90	192.0
92.00	1089.0
92.90	1624.0
94.00	3751.0
95.00	33920.0
96.00	2247.0
103.90	132.0
105.80	123.0
115.70	137.0
116.90	311.0
118.00	130.0
118.90	237.0
127.90	110.0
129.80	130.0
134.80	102.0
140.80	401.0
142.90	476.0
154.80	100.0
171.90	534.0
173.00	542.0
174.00	29416.0
175.00	2345.0
176.00	28536.0
176.90	1873.0
207.00	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB53