

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080422\
 Data File : VU050066.D
 Acq On : 04 Aug 2022 17:18
 Operator : SY/MD
 Sample : N4022-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5D55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	69	81	106	rVB3	186911	260115	53.18%	7.465%
2	1.912	170	178	196	rVB2	40638	74488	15.23%	2.138%
3	2.562	369	380	396	rVB	71481	114268	23.36%	3.279%
4	2.790	441	451	461	rBV	3798	6877	1.41%	0.197%
5	3.350	613	625	644	rVB	36580	73179	14.96%	2.100%
6	4.665	1012	1034	1064	rBV3	175592	489142	100.00%	14.038%
7	5.063	1143	1158	1176	rBV2	69647	154885	31.66%	4.445%
8	5.726	1342	1364	1389	rBV2	142825	366638	74.96%	10.522%
9	6.250	1514	1527	1546	rBV	96068	179799	36.76%	5.160%
10	6.542	1608	1618	1630	rVB6	8114	15712	3.21%	0.451%
11	6.690	1649	1664	1689	rBV	87804	175739	35.93%	5.044%
12	7.568	1923	1937	1957	rBV	40950	73825	15.09%	2.119%
13	7.899	2024	2040	2055	rBV	157441	275900	56.40%	7.918%
14	7.970	2056	2062	2073	rVB2	4992	8235	1.68%	0.236%
15	8.182	2117	2128	2144	rBV	24731	43331	8.86%	1.244%
16	8.642	2256	2271	2313	rBV5	148711	416310	85.11%	11.948%
17	9.417	2500	2512	2528	rBV	136079	228572	46.73%	6.560%
18	10.758	2916	2929	2946	rBV	75985	122955	25.14%	3.529%
19	11.812	3245	3257	3277	rBV	110420	181897	37.19%	5.220%
20	12.195	3363	3376	3394	rBV	135111	222458	45.48%	6.385%




Sum of corrected areas: 3484325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080422\
Data File : VU050066.D
Acq On : 04 Aug 2022 17:18
Operator : SY/MD
Sample : N4022-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

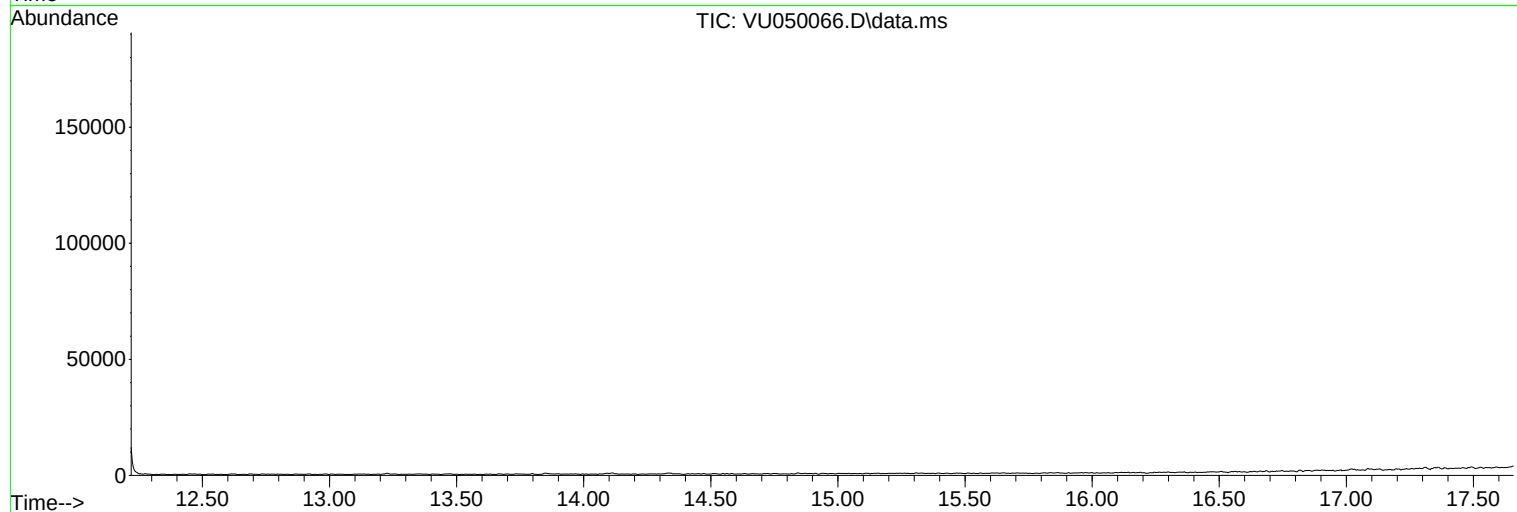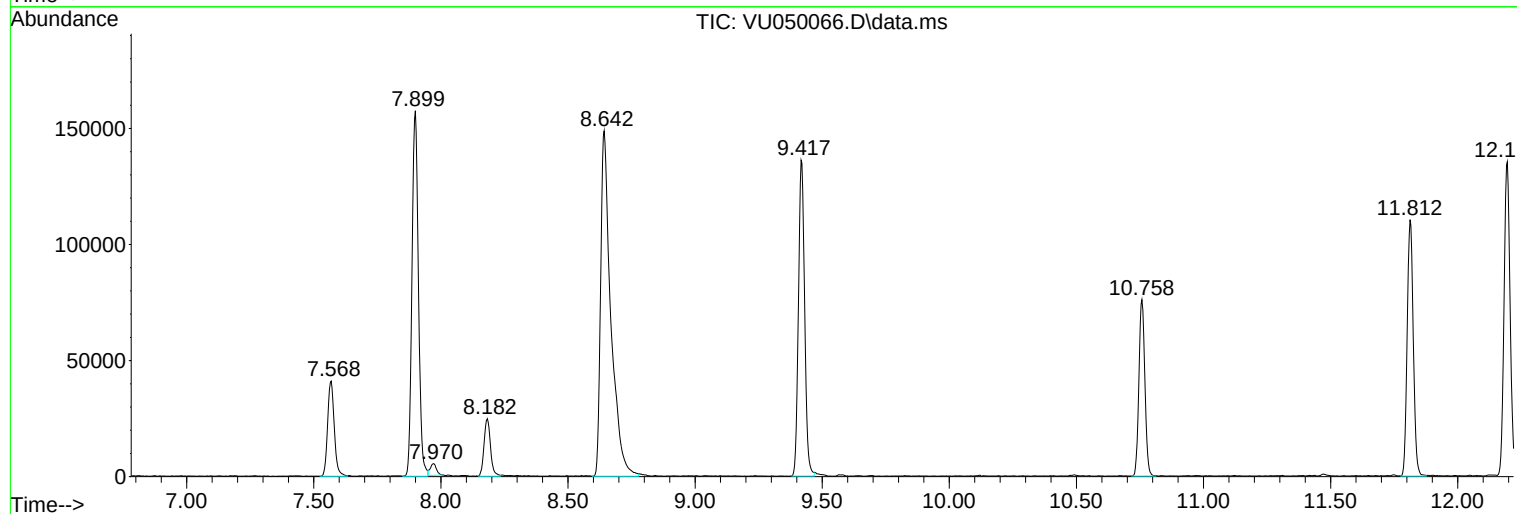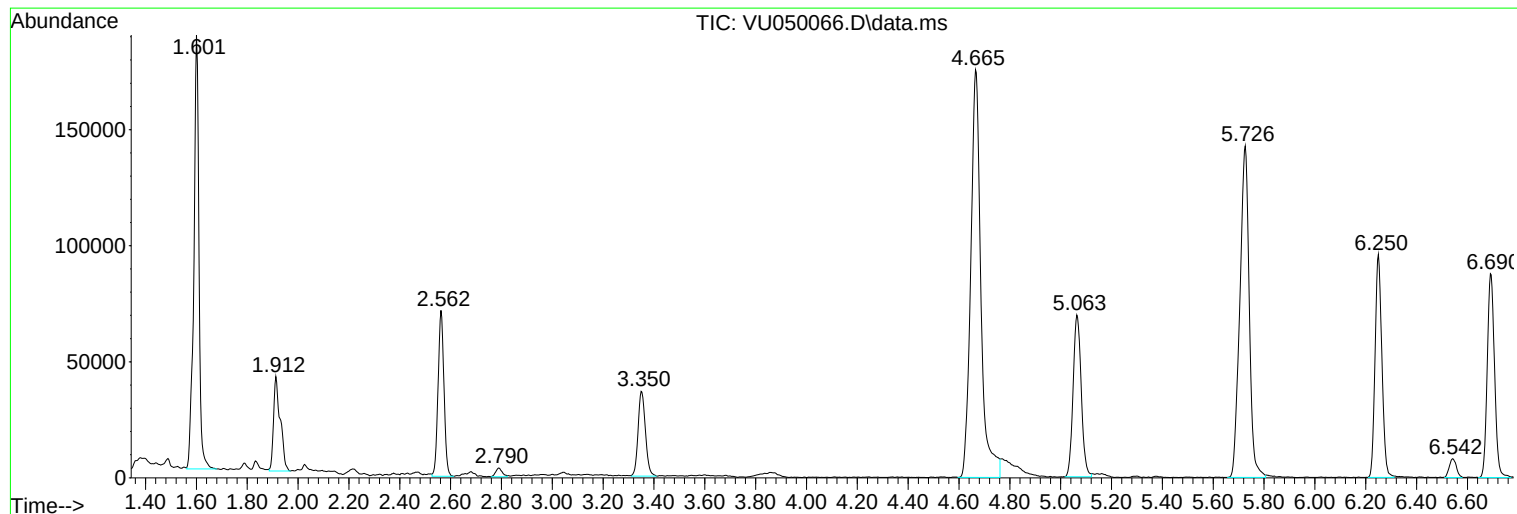

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080422\
Data File : VU050066.D
Acq On : 04 Aug 2022 17:18
Operator : SY/MD
Sample : N4022-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080422\
Data File : VU050066.D
Acq On : 04 Aug 2022 17:18
Operator : SY/MD
Sample : N4022-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc