
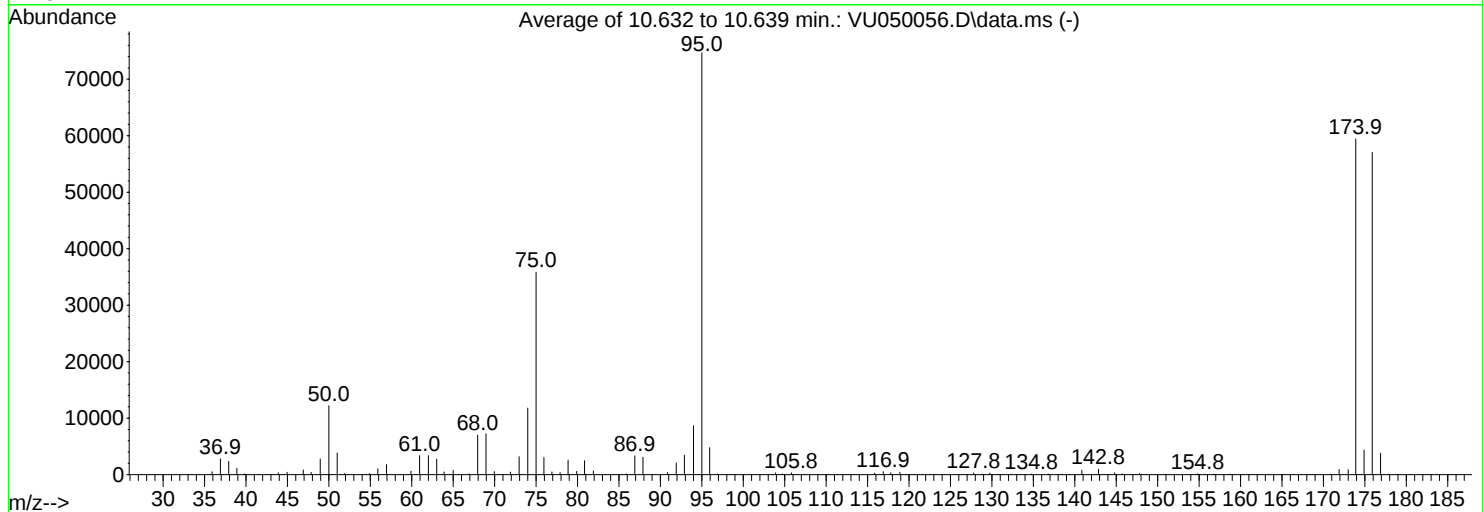


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU080422\
Data File : VU050056.D
Acq On : 04 Aug 2022 09:15
Operator : SY/MD
Sample : BFB100
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB100

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR080422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 06 06:03:36 2022

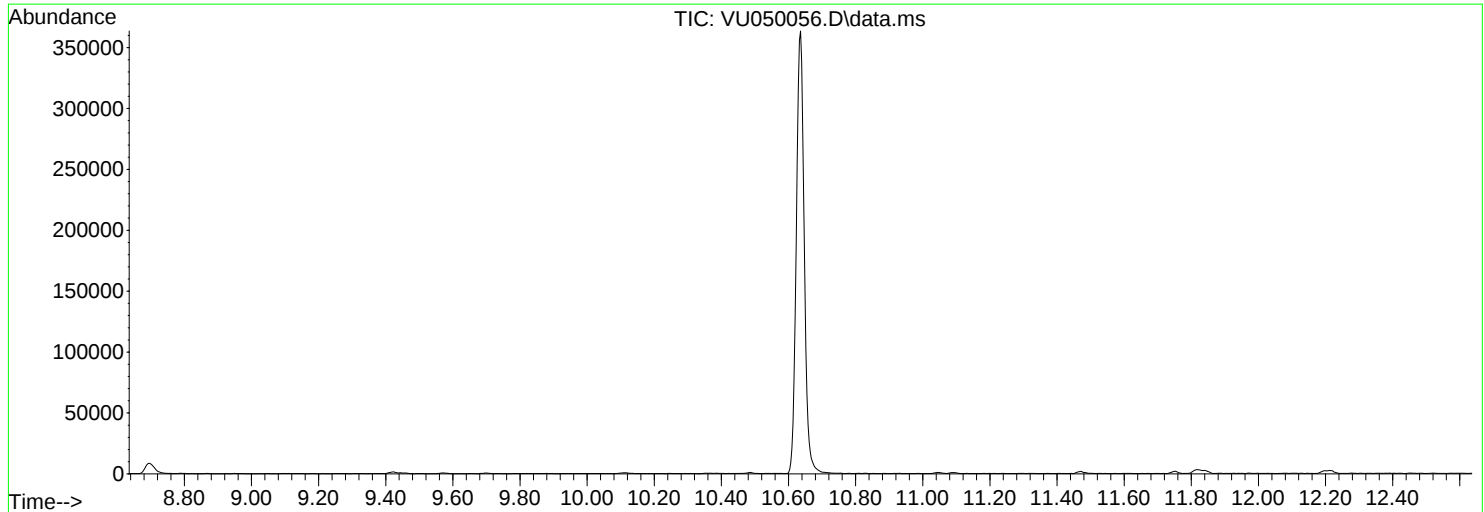

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	12217	PASS
75	95	30	80	48.0	35816	PASS
95	95	100	100	100.0	74664	PASS
96	95	5	9	6.4	4790	PASS
173	174	0.00	2	1.5	877	PASS
174	95	50	120	79.6	59427	PASS
175	174	5	9	7.3	4333	PASS
176	174	95	101	96.0	57056	PASS
177	176	5	9	6.7	3802	PASS

m/z	Abundance
43.90	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	592.0
36.90	2965.0
37.90	2443.0
38.90	1110.0
39.90	114.0
43.90	627.0
45.00	449.0
46.90	806.0
47.80	370.0
49.00	2881.0
50.00	12399.0
51.00	3991.0
51.90	196.0
52.90	127.0
54.90	210.0
55.90	1022.0
56.90	1812.0
59.90	553.0
61.00	3453.0
62.00	3429.0
63.00	2810.0
63.90	484.0
65.00	830.0
66.90	169.0
68.00	7171.0
69.00	7258.0
69.90	592.0
71.90	484.0
73.00	3202.0
74.00	11767.0
75.00	36400.0
76.00	3218.0
76.90	492.0
77.90	388.0
78.90	2697.0
79.90	622.0
80.90	2559.0
81.90	639.0
85.80	150.0
86.90	3392.0
87.90	3098.0
90.80	358.0
91.90	2106.0
92.90	3630.0
94.00	8620.0
95.00	75912.0
96.00	4919.0
96.90	167.0
103.90	320.0
104.80	110.0
105.80	325.0
115.90	226.0
116.90	577.0
117.80	341.0
118.90	444.0
127.80	294.0
129.80	286.0
130.80	106.0
134.80	150.0
136.80	153.0
140.80	789.0
142.90	1026.0
144.80	329.0
145.80	109.0
147.80	206.0
154.90	176.0
156.80	122.0
158.70	117.0
170.90	137.0
171.90	915.0
173.00	864.0
173.90	59184.0
174.90	4143.0
175.90	56856.0
176.90	3847.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	539.0
36.90	2934.0
37.90	2410.0
38.90	1122.0
39.80	151.0
43.90	616.0
44.90	436.0
46.90	862.0
47.80	423.0
48.90	2842.0
50.00	12547.0
51.00	3944.0
51.90	206.0
54.90	231.0
55.90	1071.0
56.90	1840.0
59.90	635.0
60.90	3450.0
62.00	3500.0
63.00	2788.0
63.90	477.0
65.00	782.0
66.90	191.0
68.00	7242.0
69.00	7508.0
69.90	560.0
71.90	473.0
72.90	3277.0
74.00	12174.0
75.00	36864.0
76.00	3106.0
76.90	499.0
77.90	383.0
78.80	2670.0
79.90	614.0
80.90	2496.0
81.90	707.0
85.80	168.0
86.90	3409.0
87.90	3188.0
90.90	385.0
91.90	2122.0
92.90	3560.0
94.00	8984.0
95.00	77056.0
95.90	4954.0
96.90	160.0
103.90	319.0
104.70	119.0
105.80	326.0
115.90	241.0
116.90	546.0
117.80	352.0
118.90	458.0
127.80	333.0
128.90	115.0
129.80	302.0
130.70	109.0
134.80	136.0
136.80	146.0
140.80	824.0
142.80	966.0
144.80	330.0
145.70	151.0
147.80	206.0
154.90	181.0
156.80	116.0
158.70	115.0
170.90	125.0
171.90	909.0
173.00	924.0
173.90	61296.0
174.90	4461.0
175.90	58880.0
176.90	3918.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	438.0
36.90	2529.0
37.90	2220.0
38.90	1055.0
39.90	165.0
43.90	584.0
44.90	414.0
46.90	845.0
47.90	414.0
48.90	2529.0
50.00	11704.0
51.00	3529.0
51.90	181.0
54.90	196.0
55.90	1034.0
57.00	1712.0
59.90	654.0
60.90	3196.0
62.00	3151.0
63.00	2619.0
63.90	471.0
65.00	679.0
66.90	191.0
67.90	6599.0
68.90	6953.0
70.00	488.0
71.90	405.0
72.90	3053.0
74.00	11433.0
75.00	34184.0
75.90	2756.0
76.90	477.0
77.90	308.0
78.90	2416.0
79.90	566.0
80.80	2335.0
81.90	633.0
85.90	130.0
86.90	3139.0
87.90	3002.0
90.90	373.0
91.90	1962.0
92.90	3195.0
94.00	8427.0
95.00	71024.0
95.90	4496.0
96.90	142.0
103.90	300.0
104.70	108.0
105.80	309.0
115.80	267.0
116.90	469.0
117.80	292.0
118.90	401.0
127.80	326.0
128.80	125.0
129.70	275.0
134.80	106.0
136.80	124.0
140.90	739.0
142.80	927.0
144.80	286.0
145.70	169.0
147.80	182.0
154.80	166.0
156.80	108.0
170.90	104.0
171.90	882.0
173.00	842.0
173.90	57800.0
174.90	4394.0
175.90	55432.0
176.90	3640.0
177.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100